




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025765.D
Acq On : 28 Apr 2023 17:16
Operator : SY/MD
Sample : 02526-11
Misc : 5.52g/10mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCF5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:25:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

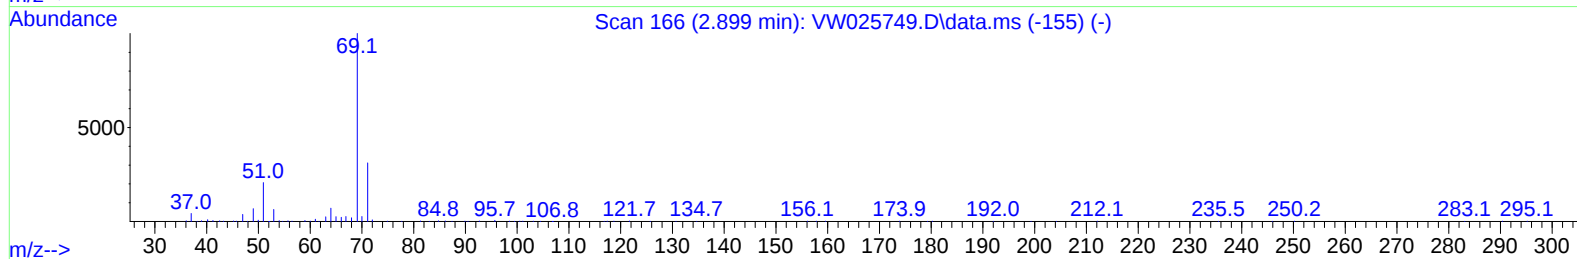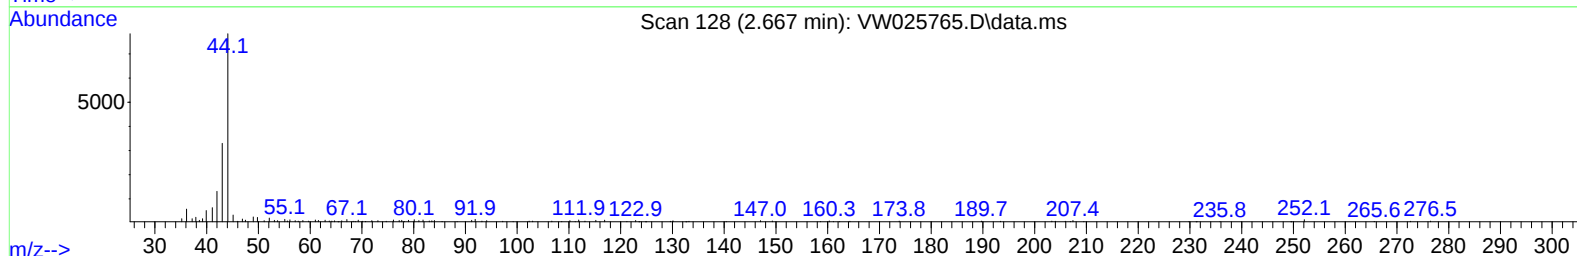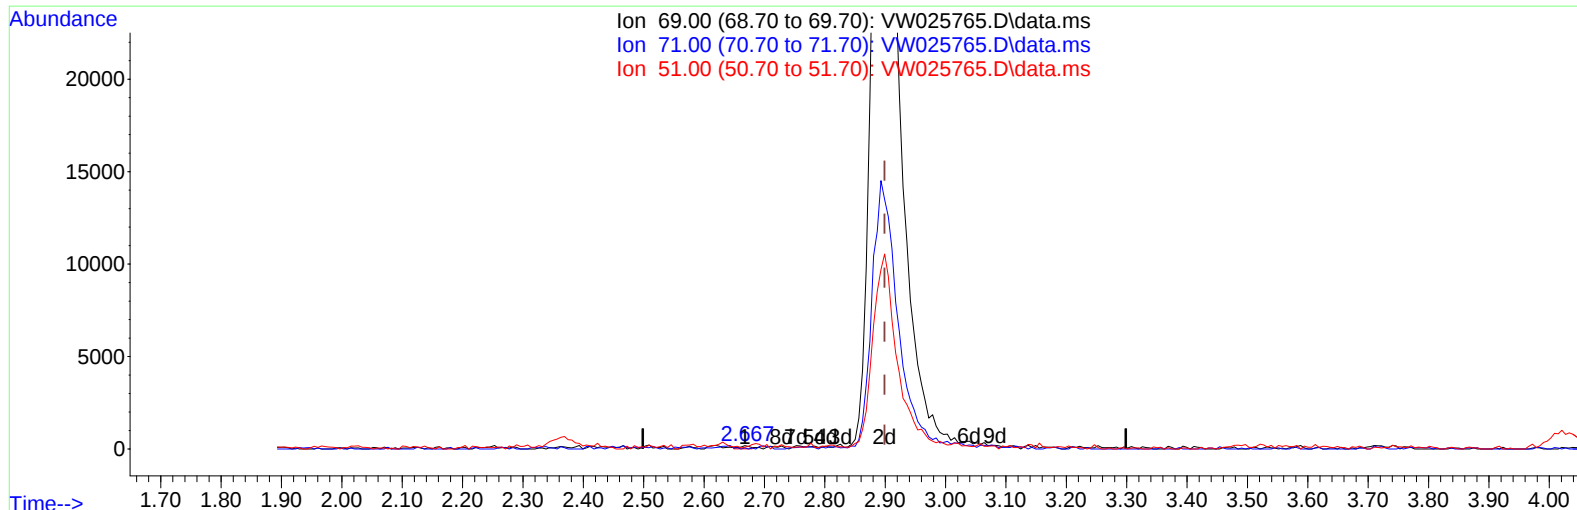

TIC: VW025765.D\data.ms

(7) Chloroethane-d5 (S)

2.667min (-0.232) 0.03 ug/L

response 193

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	23.32
51.00	13.40	17.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025765.D
 Acq On : 28 Apr 2023 17:16
 Operator : SY/MD
 Sample : 02526-11
 Misc : 5.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF5

Manual IntegrationsAPPROVED

Quant Time: Apr 29 00:25:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

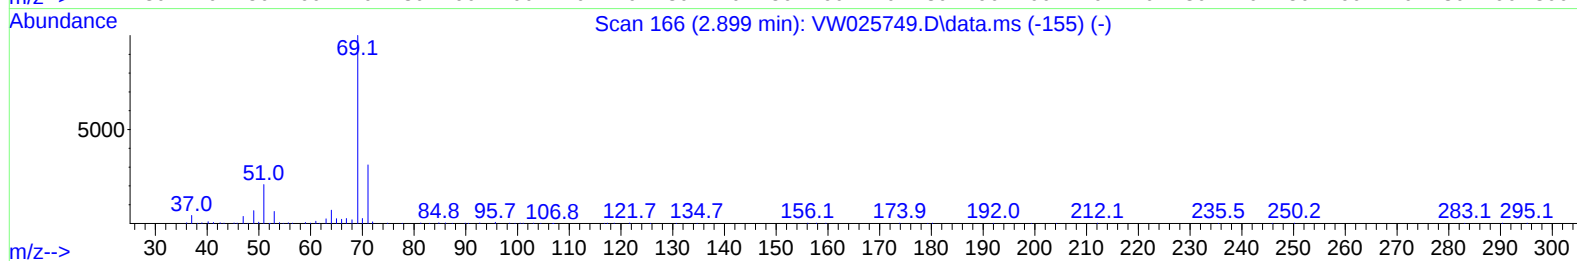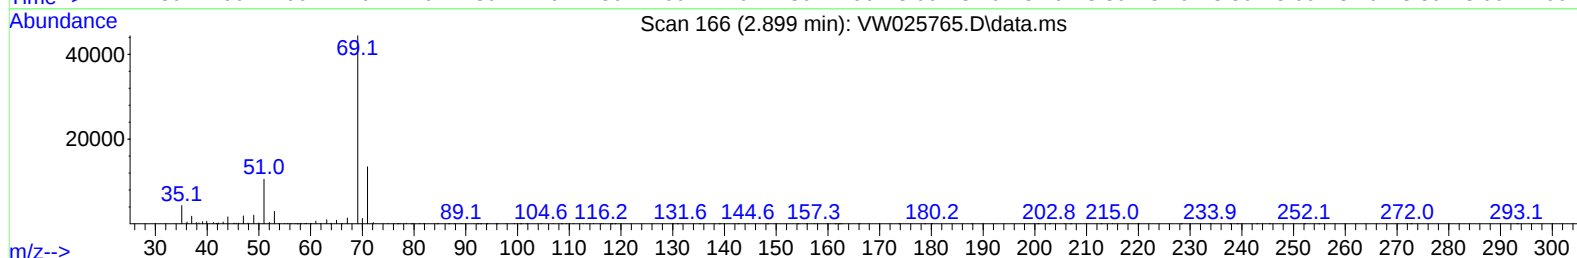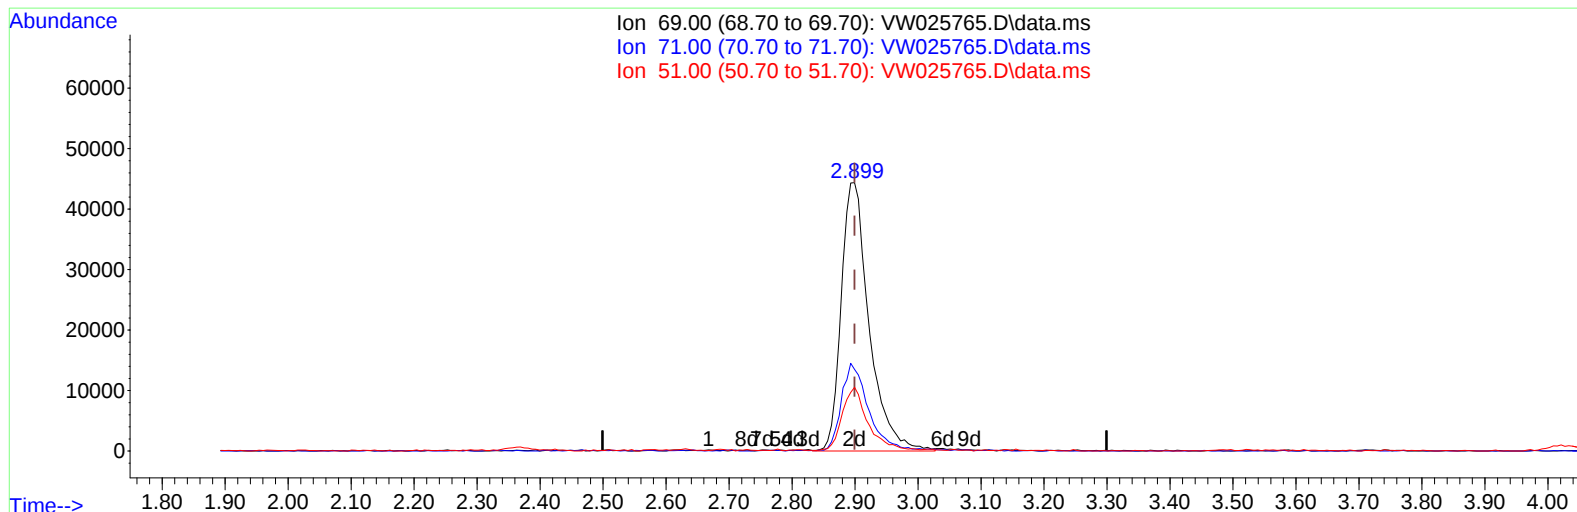

TIC: VW025765.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.000) 20.86 ug/L m

response 136591

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.03#
51.00	13.40	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025765.D
 Acq On : 28 Apr 2023 17:16
 Operator : SY/MD
 Sample : 02526-11
 Misc : 5.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCF5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:25:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	748533	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	678516	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	318483	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	158974	17.410	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	69.640%	
7) Chloroethane-d5	2.899	69	136591m	20.865	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	83.440%	
11) 1,1-Dichloroethene-d2	4.021	63	310011	14.892	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	59.560%	
21) 2-Butanone-d5	7.075	46	142389	47.256	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	94.520%	
24) Chloroform-d	7.648	84	445723	22.197	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	88.800%	
26) 1,2-Dichloroethane-d4	8.301	65	250255	22.860	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	91.440%	
32) Benzene-d6	8.276	84	861419	20.911	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	83.640%	
36) 1,2-Dichloropropane-d6	9.270	67	284186	21.328	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	85.320%	
41) Toluene-d8	10.319	98	766081	21.036	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	84.160%	
43) trans-1,3-Dichloroprop...	10.575	79	104680	20.160	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	80.640%	
47) 2-Hexanone-d5	10.922	63	98704	47.695	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	95.400%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	222219	22.629	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	90.520%	
66) 1,2-Dichlorobenzene-d4	13.848	152	250427	22.951	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	91.800%	
Target Compounds						
					Qvalue	
13) Acetone	4.112	43	366364	131.177	ug/L	100
22) 2-Butanone	7.167	43	21650	6.114	ug/L	96
46) Tetrachloroethene	10.861	164	8902	1.051	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025765.D
Acq On : 28 Apr 2023 17:16
Operator : SY/MD
Sample : 02526-11
Misc : 5.52g/10mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCF5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:25:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

