

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
 Data File : VW025755.D
 Acq On : 28 Apr 2023 13:17
 Operator : SY/MD
 Sample : 02526-20
 Misc : 3.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCL4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 29 00:23:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 28 02:55:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	675103	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	601717	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	283244	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	168148	20.418	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.680%		
7) Chloroethane-d5	2.899	69	138924	23.529	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.120%		
11) 1,1-Dichloroethene-d2	4.021	63	311950	16.615	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.440%		
21) 2-Butanone-d5	7.075	46	146455	53.893	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	107.780%		
24) Chloroform-d	7.648	84	455607	25.157	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	100.640%		
26) 1,2-Dichloroethane-d4	8.307	65	259282m	26.261	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	105.040%		
32) Benzene-d6	8.276	84	878658	24.052	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	96.200%		
36) 1,2-Dichloropropane-d6	9.270	67	289990	24.541	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.160%		
41) Toluene-d8	10.319	98	768431	23.794	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	95.160%		
43) trans-1,3-Dichloroprop...	10.575	79	109383	23.754	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	95.000%		
47) 2-Hexanone-d5	10.922	63	99443	54.185	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.380%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	222408	25.539	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.160%		
66) 1,2-Dichlorobenzene-d4	13.848	152	261798	26.978	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	107.920%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	147840	58.692	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042823\
Data File : VW025755.D
Acq On : 28 Apr 2023 13:17
Operator : SY/MD
Sample : 02526-20
Misc : 3.75g/10mL/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DCCL4

Quant Time: Apr 29 00:23:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM042723SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 28 02:55:08 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/29/2023
Supervised By :Mahesh Dadoda 05/01/2023

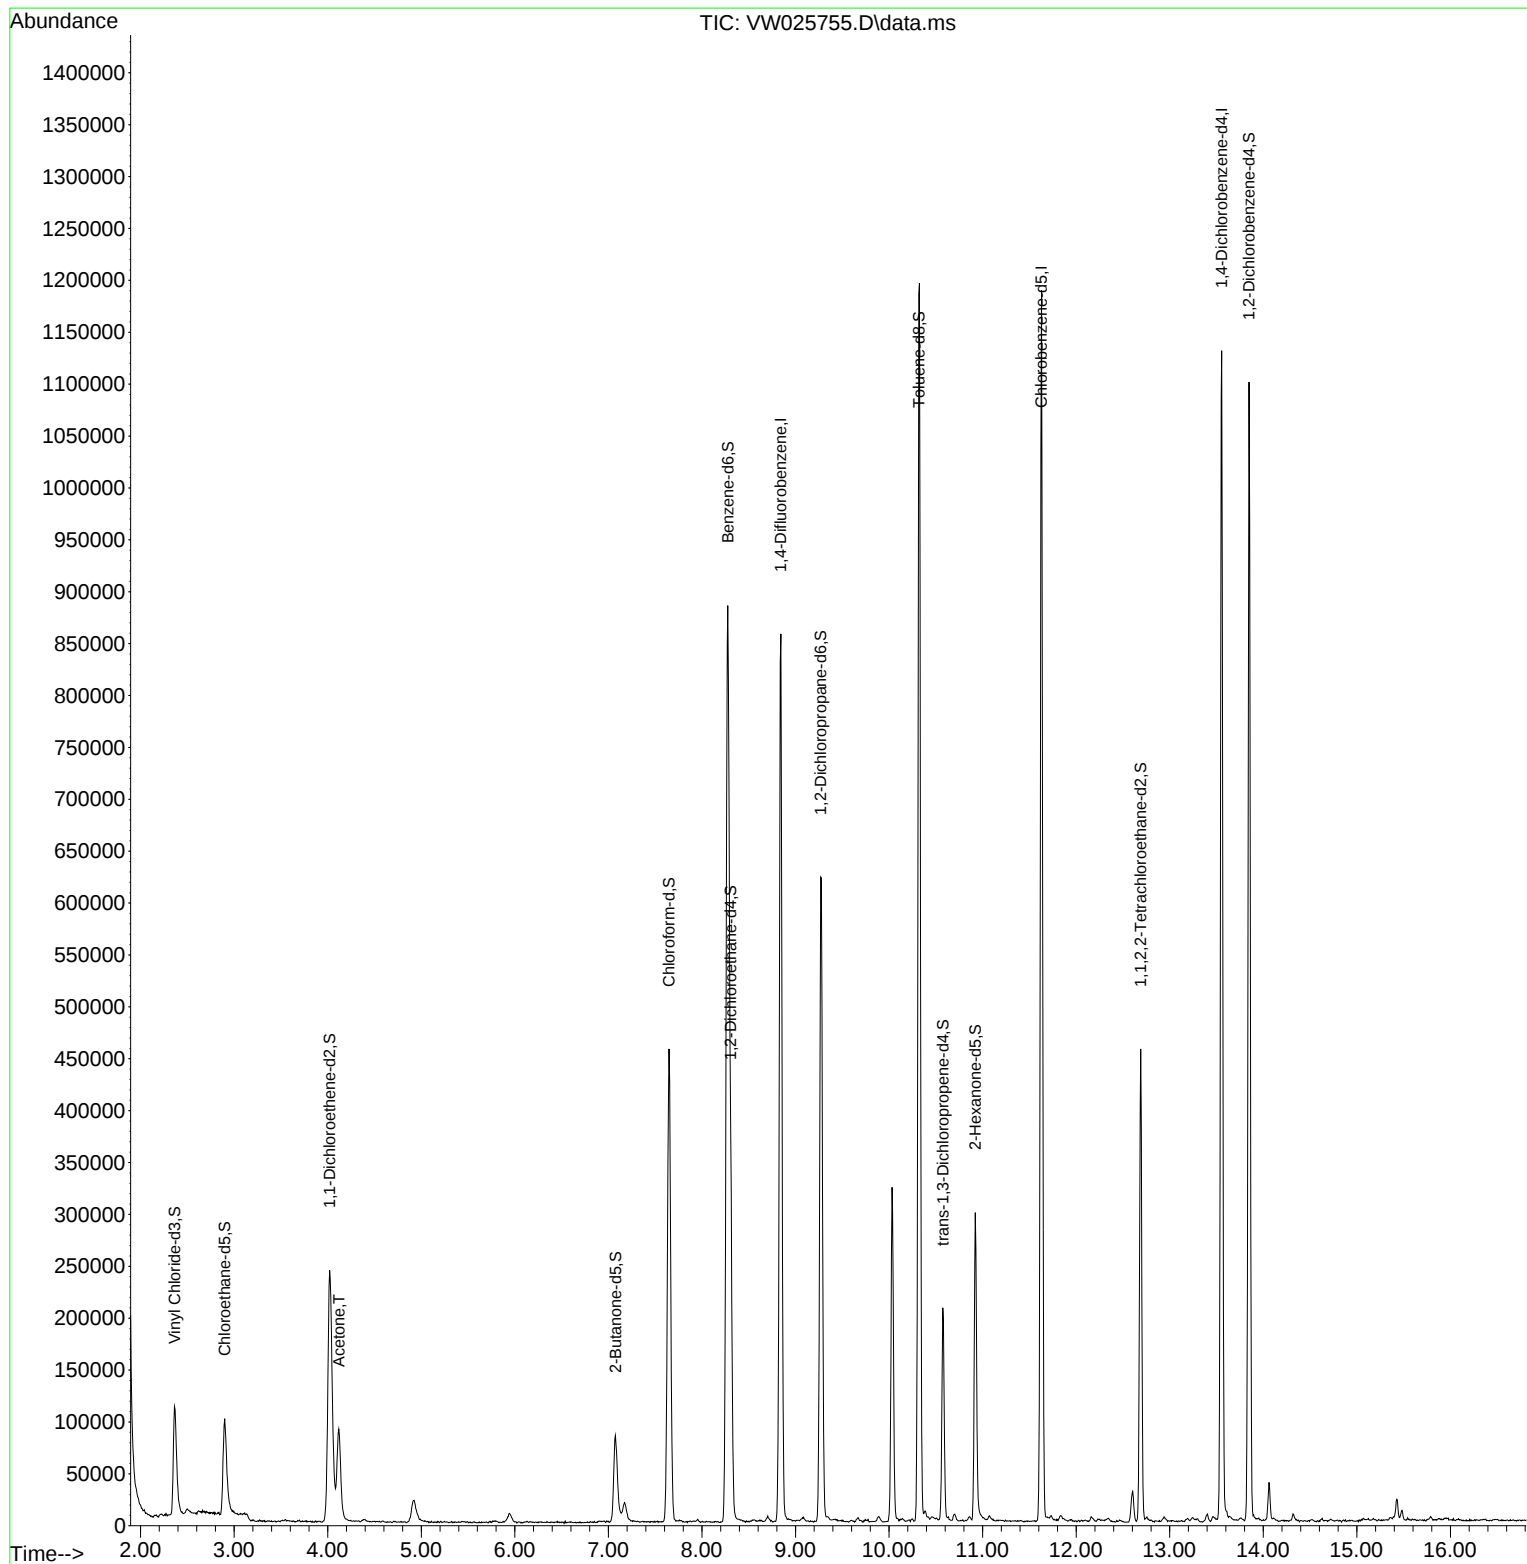

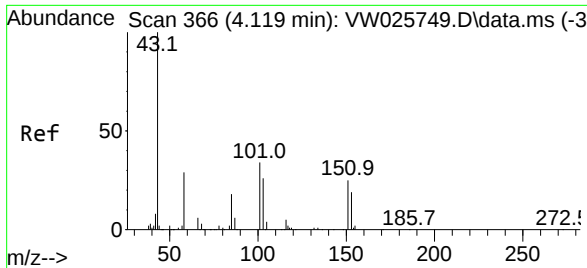

#13
 Acetone
 Concen: 58.692 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW025755.D
 Acq: 28 Apr 2023 13:17

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCL4

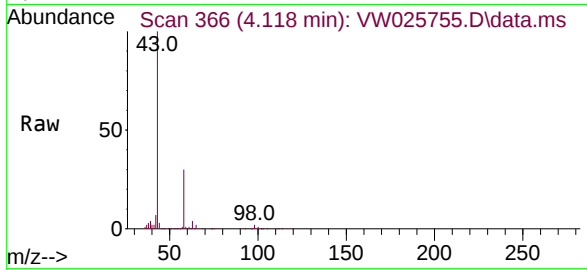

Tgt Ion: 43 Resp: 147840
 Ion Ratio Lower Upper
 43 100
 58 30.0 0.0 58.6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/29/2023
 Supervised By :Mahesh Dadoda 05/01/2023

