

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022712.D
 Acq On : 29 Apr 2022 21:41
 Operator : SY/VA
 Sample : N2638-01
 Misc : 6.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 30 02:00:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	266915	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	238461	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93625	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	114177	19.350	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.400%
7) Chloroethane-d5	2.885	69	78698	21.281	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.120%
11) 1,1-Dichloroethene-d2	4.019	63	124828	16.310	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.240%
21) 2-Butanone-d5	7.079	46	48067	46.659	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.320%
24) Chloroform-d	7.646	84	207789	24.906	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.640%
26) 1,2-Dichloroethane-d4	8.189	65	95	0.020	ug/L	-0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.274	84	388173	26.644	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	106.560%
36) 1,2-Dichloropropane-d6	9.274	67	116596	27.655	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.600%
41) Toluene-d8	10.323	98	343023	24.040	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.160%
43) trans-1,3-Dichloroprop...	10.573	79	41662	20.938	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.760%
47) 2-Hexanone-d5	10.920	63	38320	48.851	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.700%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	98237	27.403	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	82825	24.976	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.920%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.042	75	3449	0.560	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022712.D
Acq On : 29 Apr 2022 21:41
Operator : SY/VA
Sample : N2638-01
Misc : 6.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 30 02:00:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 30 01:41:13 2022
Response via : Initial Calibration

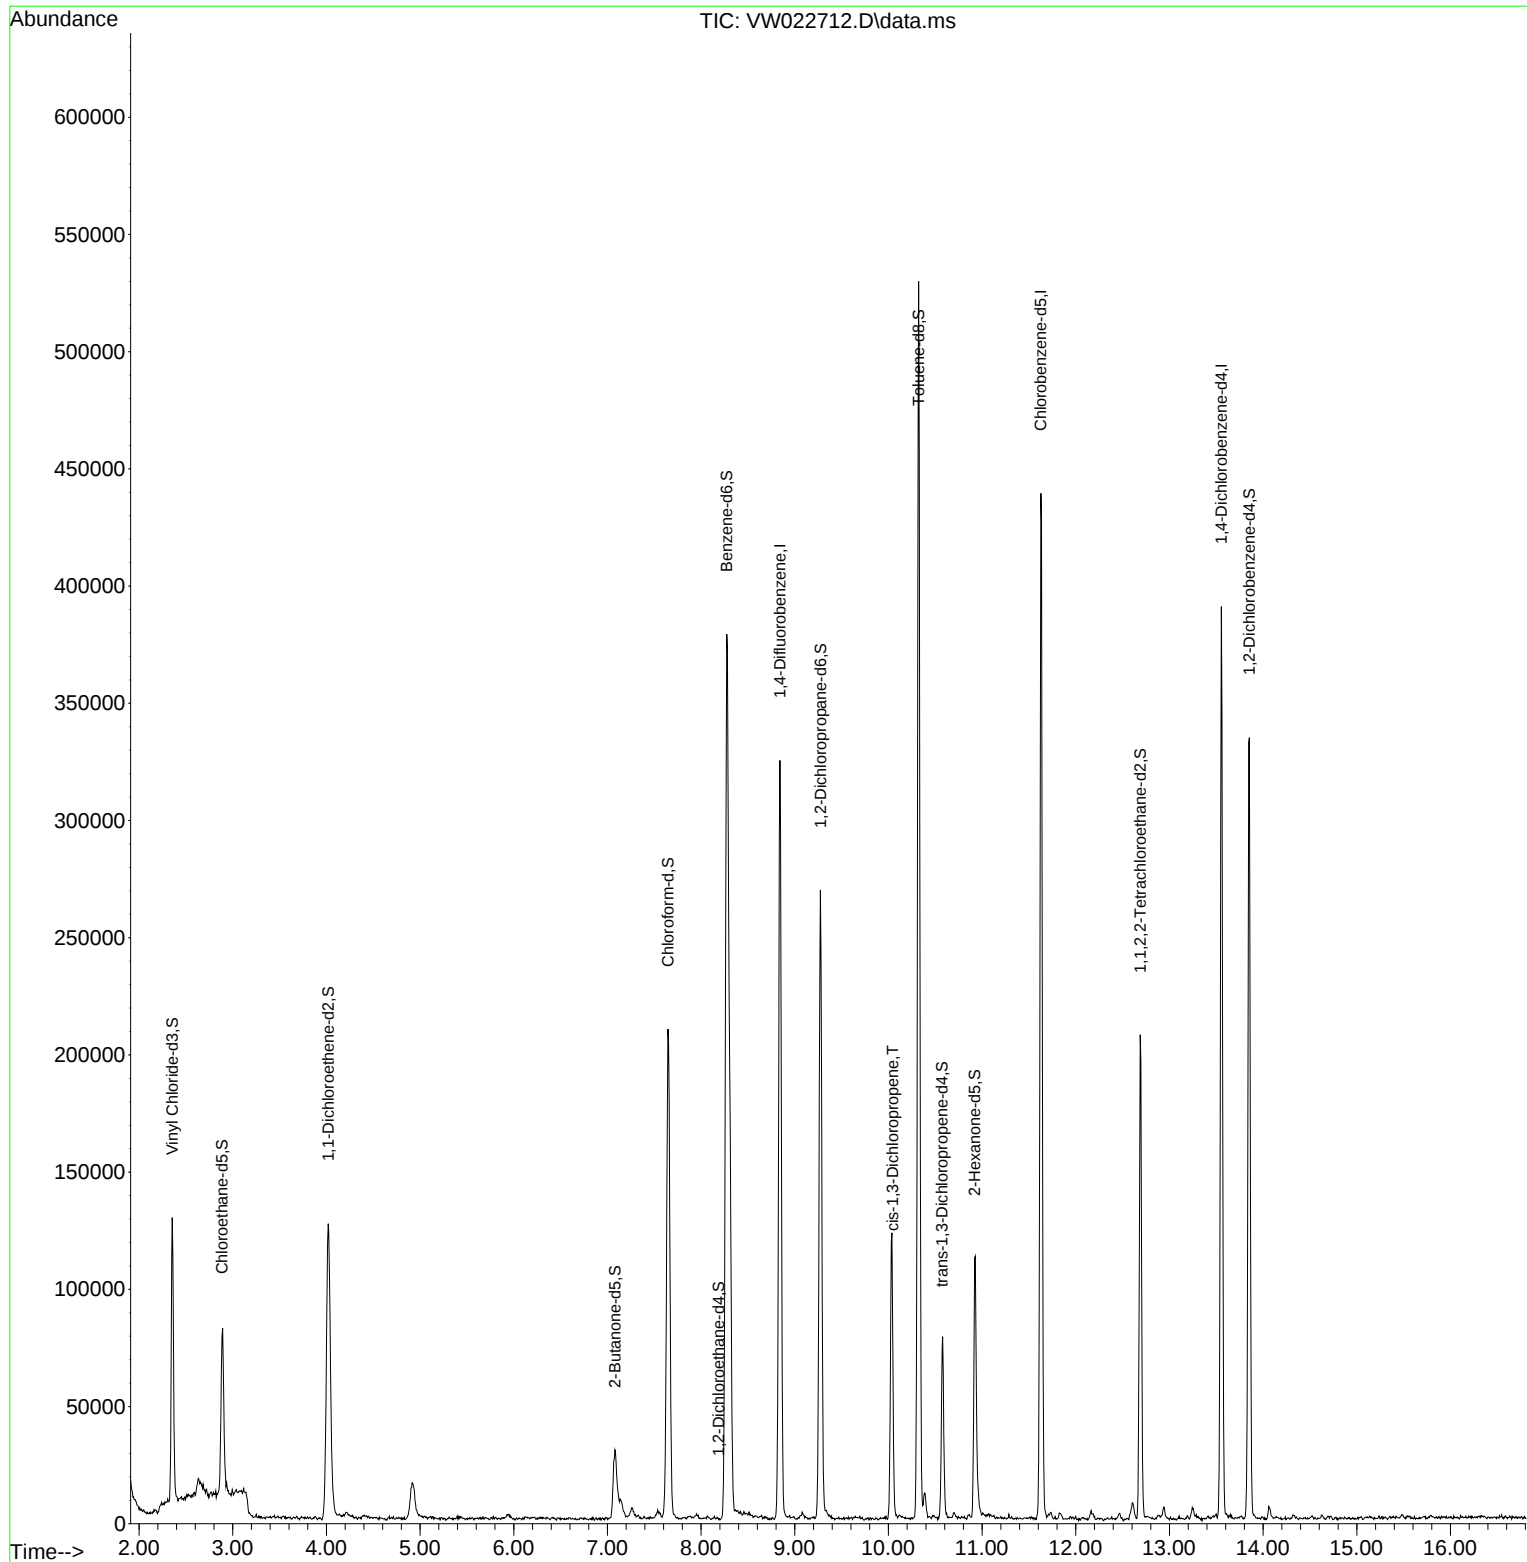

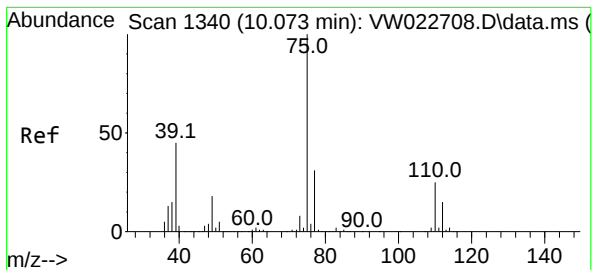

#39
 cis-1,3-Dichloropropene
 Concen: 0.560 ug/L
 RT: 10.042 min Scan# 11
 Delta R.T. -0.031 min
 Lab File: VW022712.D
 Acq: 29 Apr 2022 21:41

Instrument :
 MSVOA_W
 ClientSampleId :

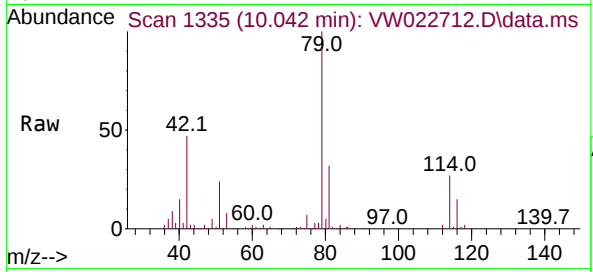

Tgt Ion: 75 Resp: 3449
 Ion Ratio Lower Upper
 75 100
 77 41.4 22.6 42.0

