

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022714.D
 Acq On : 29 Apr 2022 22:29
 Operator : SY/VA
 Sample : N2638-05
 Misc : 4.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 30 02:01:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	259036	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	257868	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	127766	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	116232	20.297	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.200%
7) Chloroethane-d5	2.885	69	79988	22.288	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.160%
11) 1,1-Dichloroethene-d2	4.202	63	120	0.016	ug/L	0.18
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.080%#
21) 2-Butanone-d5	7.080	46	51465	51.477	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.960%
24) Chloroform-d	7.647	84	214232	26.460	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.840%
26) 1,2-Dichloroethane-d4	8.384	65	191	0.041	ug/L	0.08
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.275	84	407086	25.839	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.360%
36) 1,2-Dichloropropane-d6	9.274	67	119825	26.282	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.120%
41) Toluene-d8	10.323	98	373435	24.202	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.800%
43) trans-1,3-Dichloroprop...	10.579	79	46213	21.477	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.920%
47) 2-Hexanone-d5	10.921	63	44205	52.113	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.220%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	103158	26.610	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	120894	26.714	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.840%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	3994	0.600	ug/L #	73
46) Tetrachloroethene	10.860	164	12858	3.731	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022714.D
Acq On : 29 Apr 2022 22:29
Operator : SY/VA
Sample : N2638-05
Misc : 4.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 30 02:01:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 30 01:41:13 2022
Response via : Initial Calibration

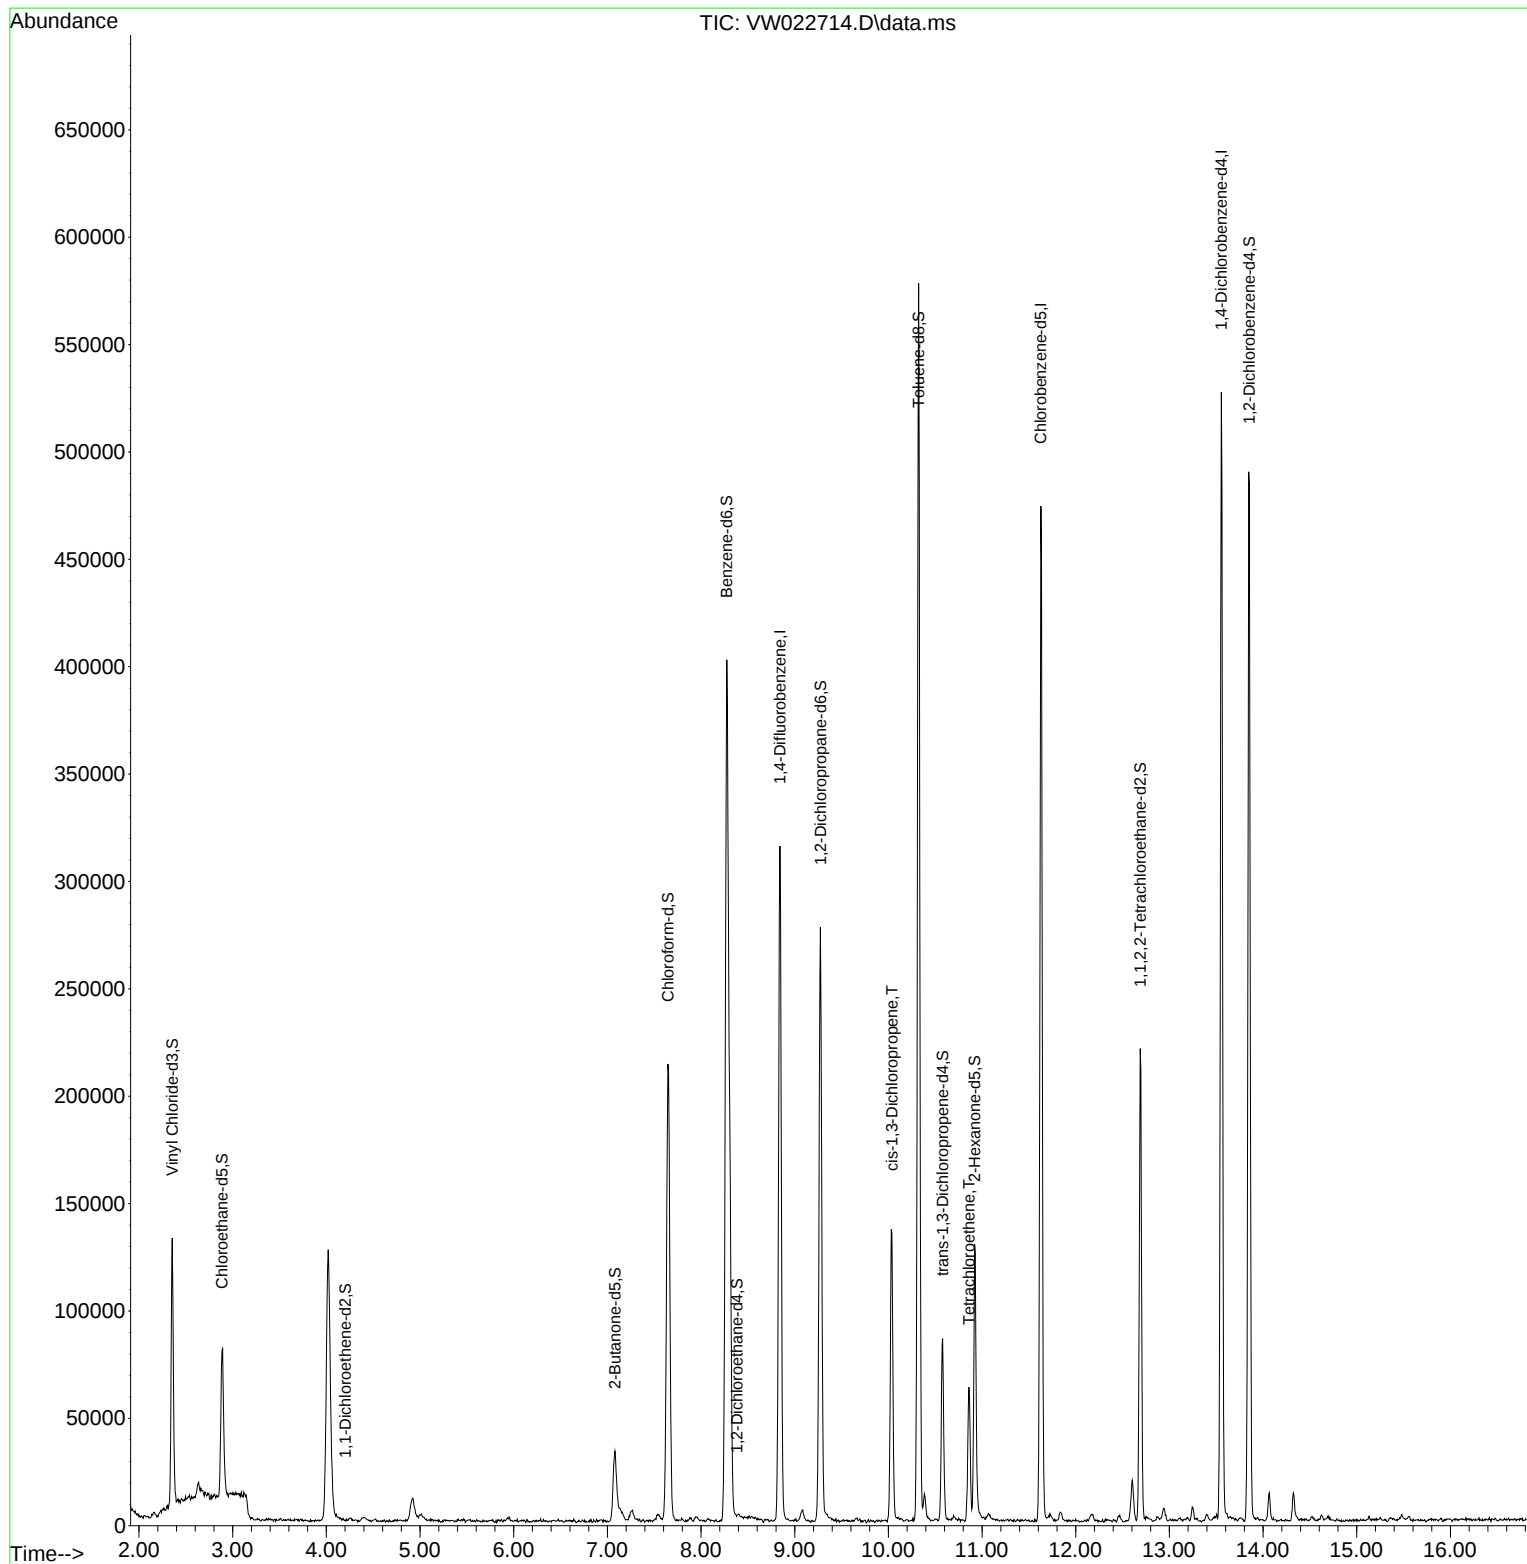

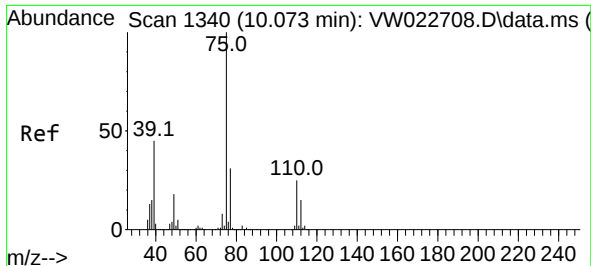

#39

cis-1,3-Dichloropropene

Concen: 0.600 ug/L

RT: 10.037 min Scan# 1

Delta R.T. -0.037 min

Lab File: VW022714.D

Acq: 29 Apr 2022 22:29

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 75 Resp: 3994

Ion Ratio Lower Upper

75 100

77 47.3 22.6 42.0#

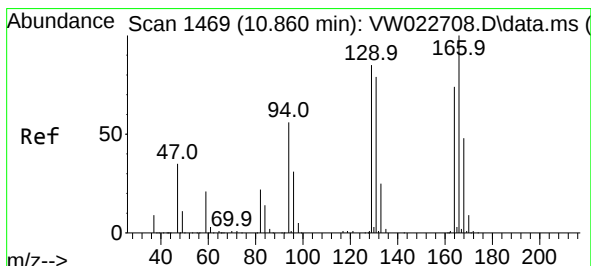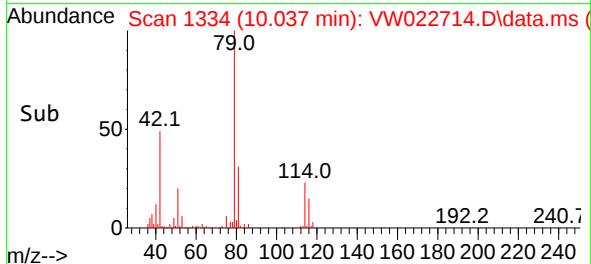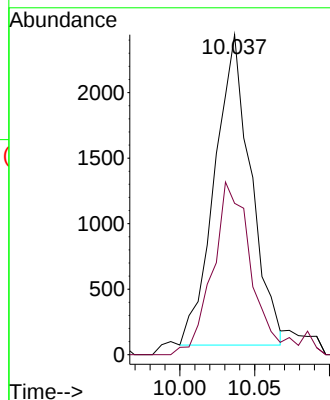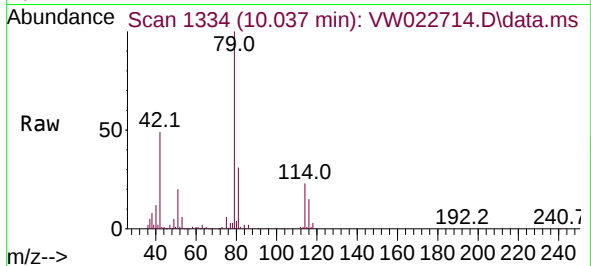

#46

Tetrachloroethene

Concen: 3.731 ug/L

RT: 10.860 min Scan# 1469

Delta R.T. -0.000 min

Lab File: VW022714.D

Acq: 29 Apr 2022 22:29

Tgt Ion: 164 Resp: 12858

Ion Ratio Lower Upper

164 100

129 96.1 74.1 137.7

131 99.7 71.4 132.6

166 143.0 95.9 178.1

