

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022718.D
 Acq On : 30 Apr 2022 00:06
 Operator : SY/VA
 Sample : N2638-14
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 30 02:01:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	254272	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	224596	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	86770	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	103847	18.474	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.880%
7) Chloroethane-d5	2.885	69	74184	21.058	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.240%
11) 1,1-Dichloroethene-d2	4.013	63	107280	14.714	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.840%
21) 2-Butanone-d5	7.079	46	48679	49.602	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.200%
24) Chloroform-d	7.646	84	189511	23.845	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.360%
26) 1,2-Dichloroethane-d4	8.305	65	115229	25.375	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.520%
32) Benzene-d6	8.274	84	341282	24.871	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.480%
36) 1,2-Dichloropropane-d6	9.268	67	107922	27.178	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.720%
41) Toluene-d8	10.323	98	303596	22.590	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.360%
43) trans-1,3-Dichloroprop...	10.573	79	34732	18.533	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.120%
47) 2-Hexanone-d5	10.920	63	35656	48.261	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.520%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103813	30.746	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	123.000%#
66) 1,2-Dichlorobenzene-d4	13.853	152	75401	24.533	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.120%
Target Compounds						
39) cis-1,3-Dichloropropene	10.030	75	3298	0.569	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022718.D
Acq On : 30 Apr 2022 00:06
Operator : SY/VA
Sample : N2638-14
Misc : 5.61g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 30 02:01:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 30 01:41:13 2022
Response via : Initial Calibration

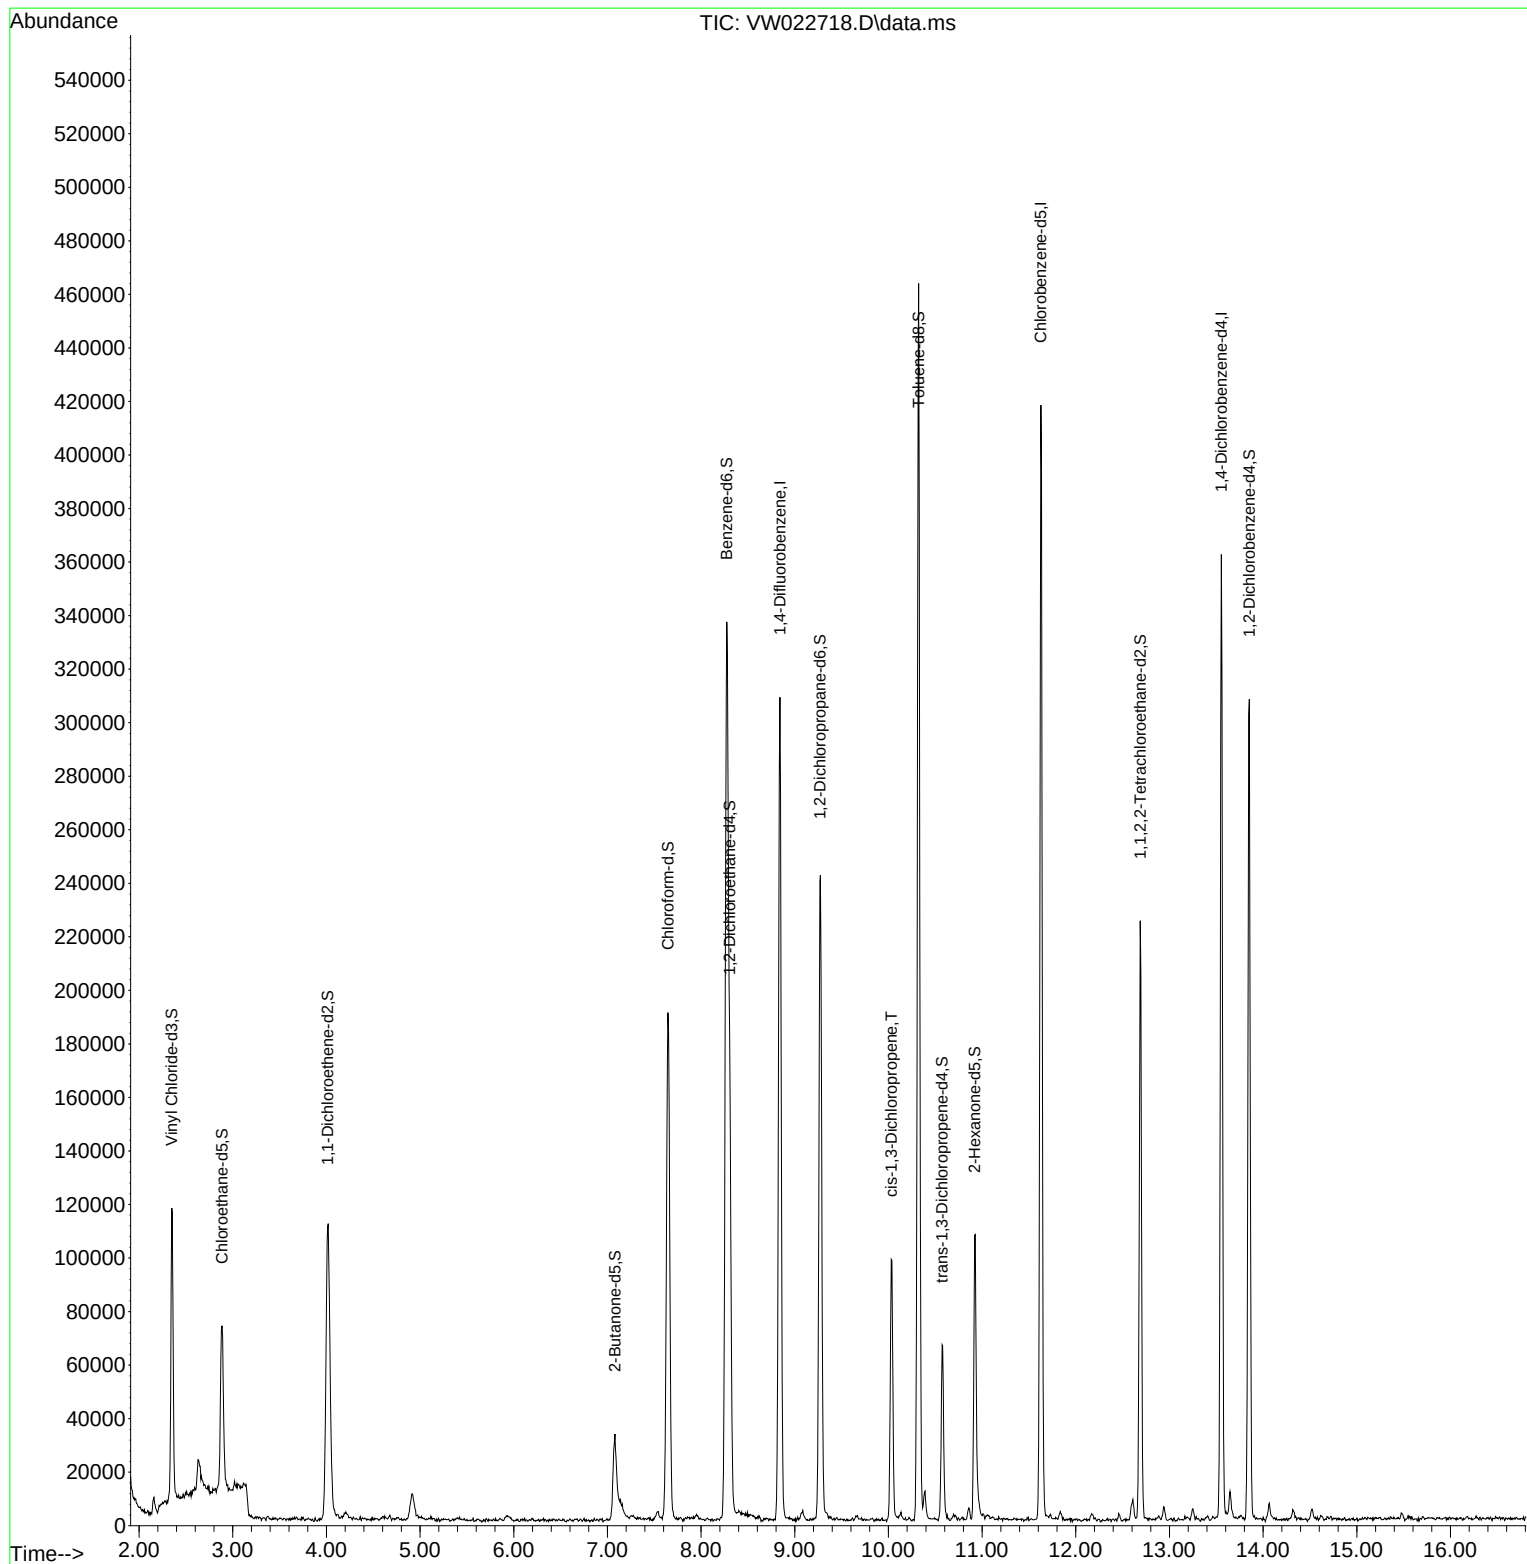

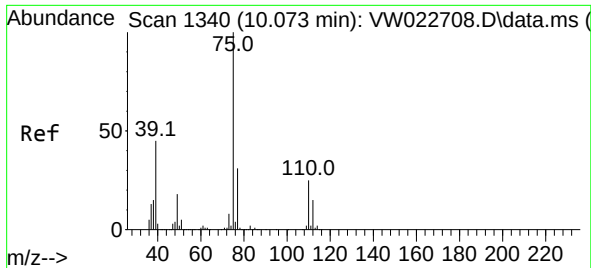

#39
 cis-1,3-Dichloropropene
 Concen: 0.569 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VW022718.D
 Acq: 30 Apr 2022 00:06

Instrument :
 MSVOA_W
 ClientSampleId :

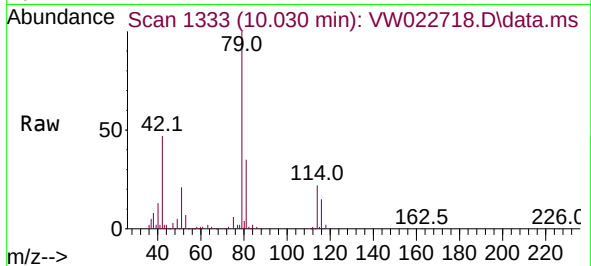

Tgt Ion: 75 Resp: 3298
 Ion Ratio Lower Upper
 75 100
 77 41.8 22.6 42.0

