




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022690.D
 Acq On : 29 Apr 2022 11:09
 Operator : SY/VA
 Sample : N2603-09RE
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW490RE

Manual IntegrationsAPPROVED

Quant Time: Apr 29 22:23:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

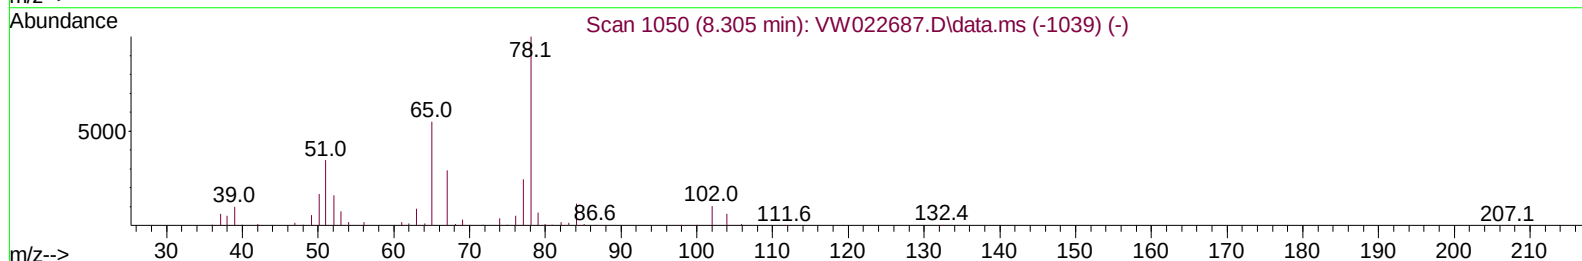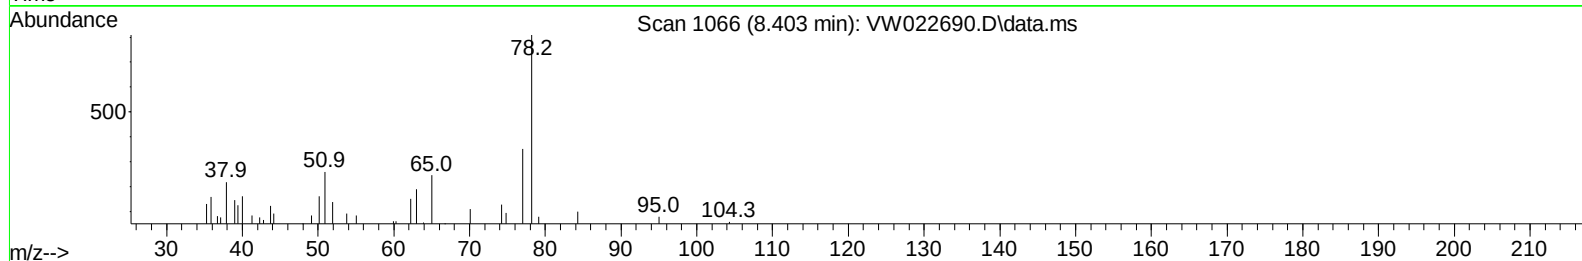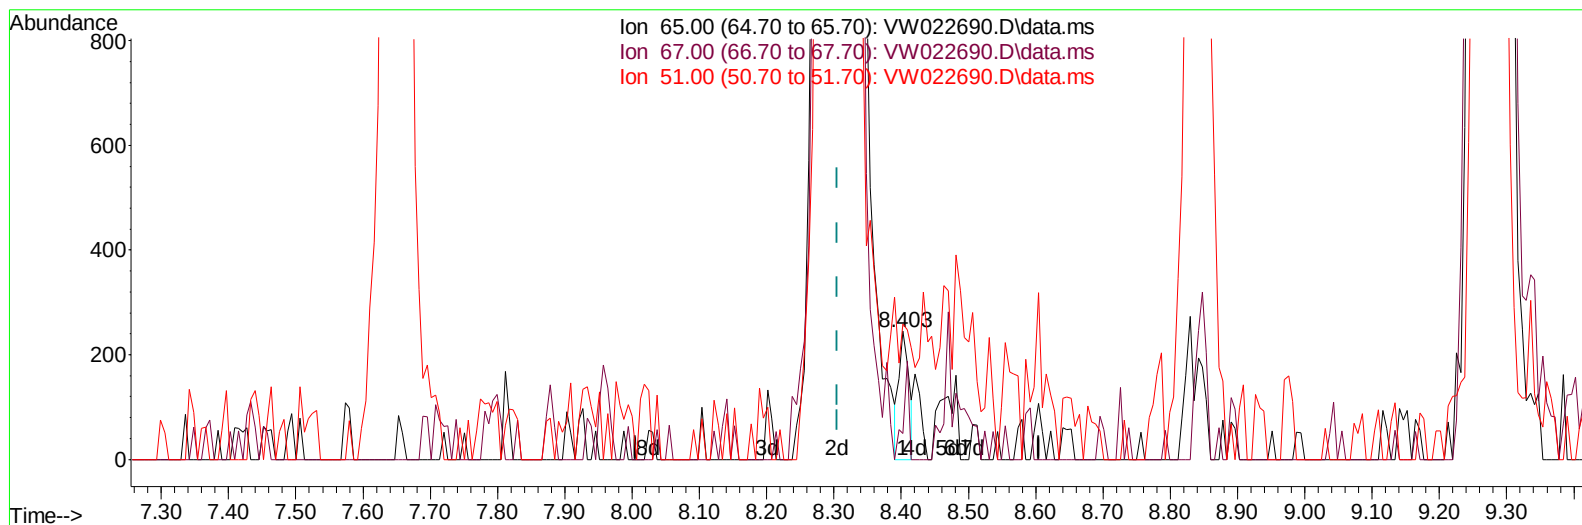

TIC: VW022690.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+ 0.098) 0.06 ug/L

response 255

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	42.35
51.00	99.30	80.78
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022690.D
 Acq On : 29 Apr 2022 11:09
 Operator : SY/VA
 Sample : N2603-09RE
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW490RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:23:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

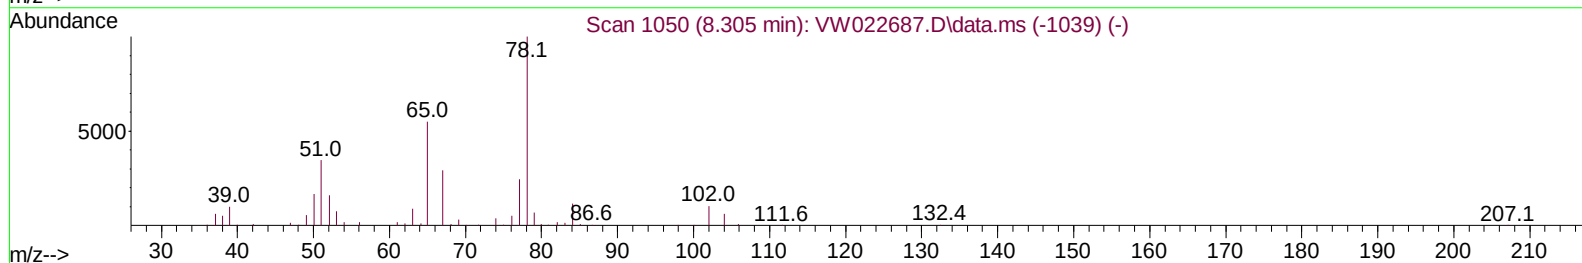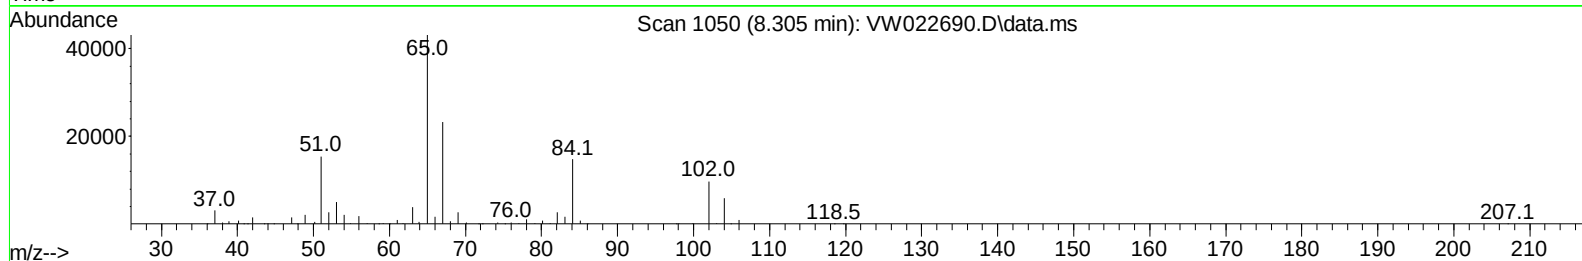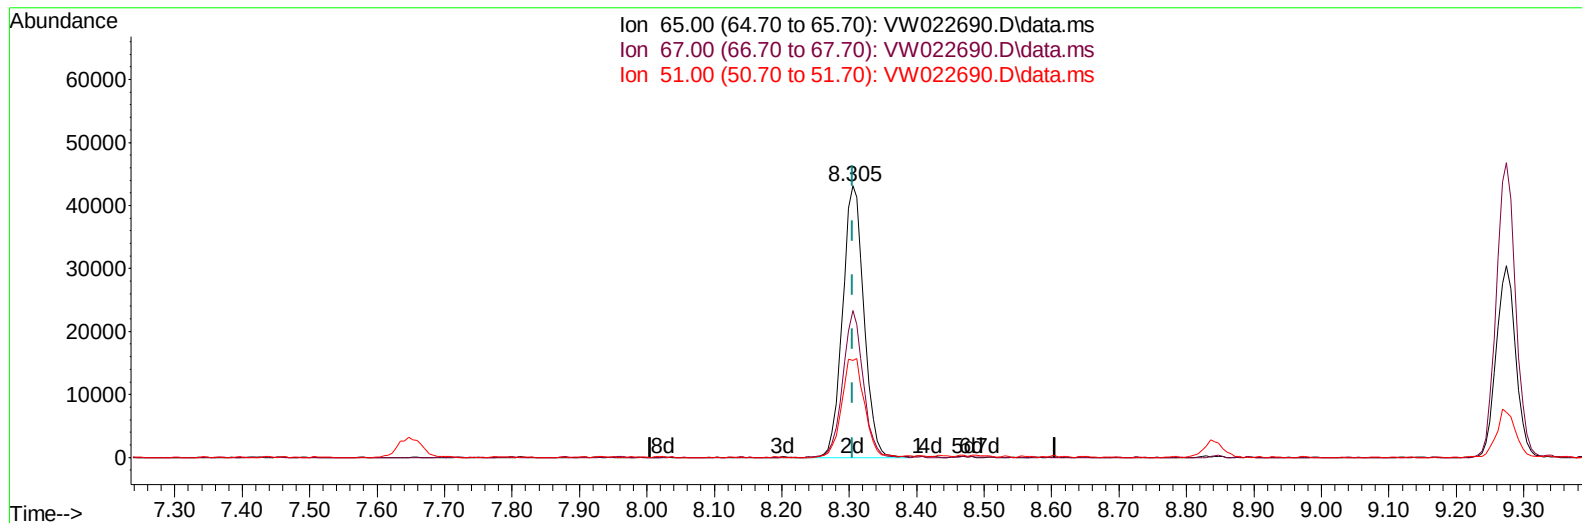

TIC: VW022690.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 22.02 ug/L m

response 94757

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.11#
51.00	99.30	0.22#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022690.D
 Acq On : 29 Apr 2022 11:09
 Operator : SY/VA
 Sample : N2603-09RE
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW490RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:23:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	240912	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	120162	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	19135	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	74845	14.053	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.200%	
7) Chloroethane-d5	2.885	69	66198	19.833	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	79.320%	
11) 1,1-Dichloroethene-d2	4.019	63	79681	11.535	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	46.160%	
21) 2-Butanone-d5	7.080	46	71409	76.799	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	153.600%#	
24) Chloroform-d	7.653	84	178374	23.688	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	94.760%	
26) 1,2-Dichloroethane-d4	8.305	65	94757m	22.024	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	88.080%	
32) Benzene-d6	8.275	84	276082	37.606	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	150.440%#	
36) 1,2-Dichloropropane-d6	9.274	67	93164	43.852	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	175.400%#	
41) Toluene-d8	10.323	98	169566	23.583	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	94.320%	
43) trans-1,3-Dichloroprop...	10.579	79	19844	19.791	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.160%	
47) 2-Hexanone-d5	10.927	63	42741	108.130	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	216.260%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85282	47.210	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	188.840%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	19248	28.399	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	113.600%	
Target Compounds						
13) Acetone	4.135	43	4962	7.838	ug/L	89
14) Carbon disulfide	4.391	76	13545	1.269	ug/L	96
42) Toluene	10.390	91	13400	1.433	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022690.D
Acq On : 29 Apr 2022 11:09
Operator : SY/VA
Sample : N2603-09RE
Misc : 5.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW490RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:23:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

