




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022692.D
Acq On : 29 Apr 2022 11:57
Operator : SY/VA
Sample : N2603-11
Misc : 7.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW492

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

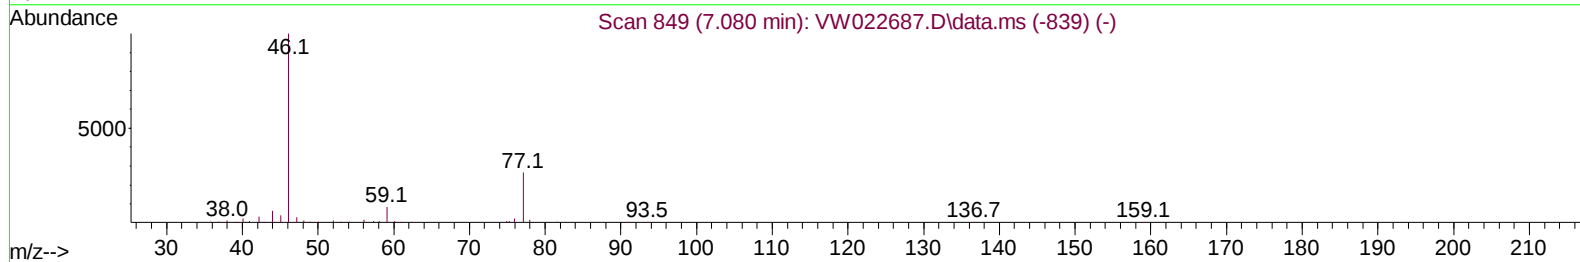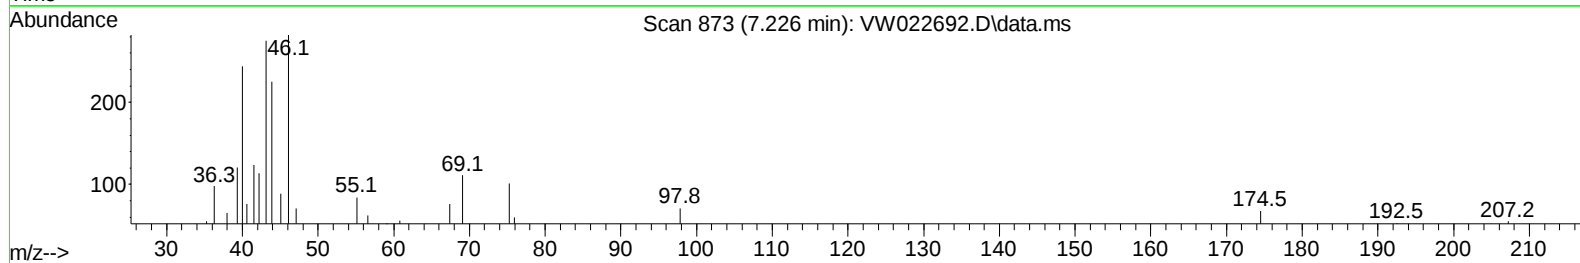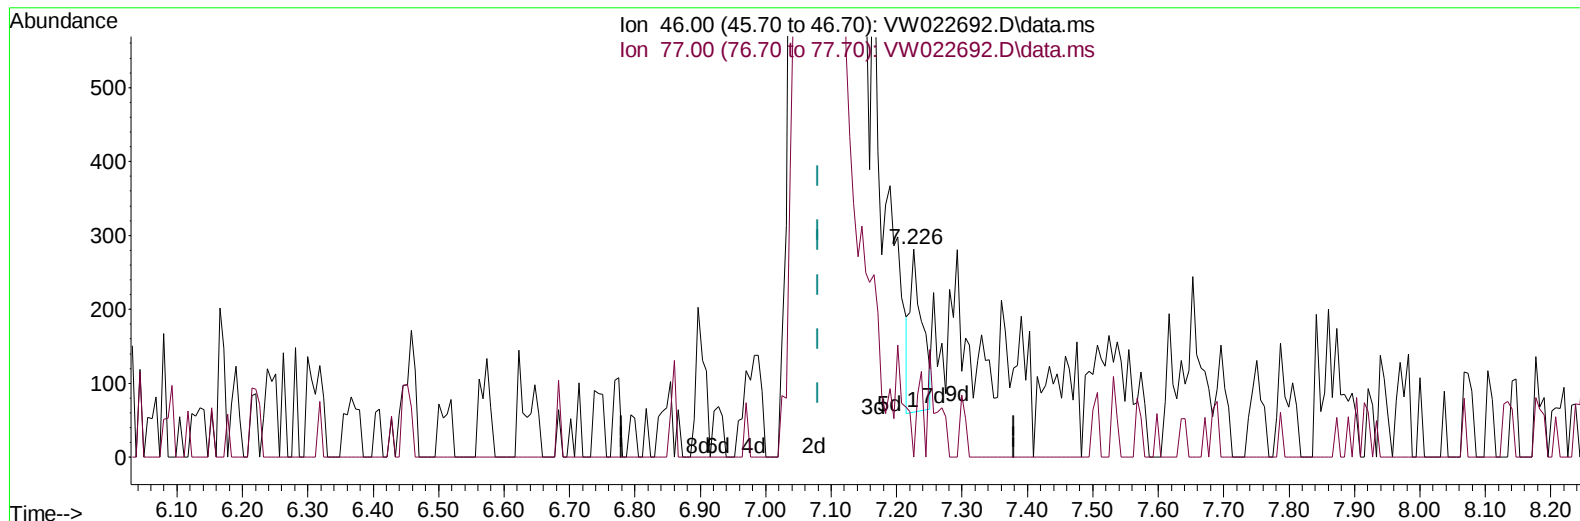

TIC: VW022692.D\data.ms

(21) 2-Butanone-d5 (S)

7.226min (+ 0.146) 0.24 ug/L

response 287

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	25.44
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022692.D
 Acq On : 29 Apr 2022 11:57
 Operator : SY/VA
 Sample : N2603-11
 Misc : 7.71g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW492

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

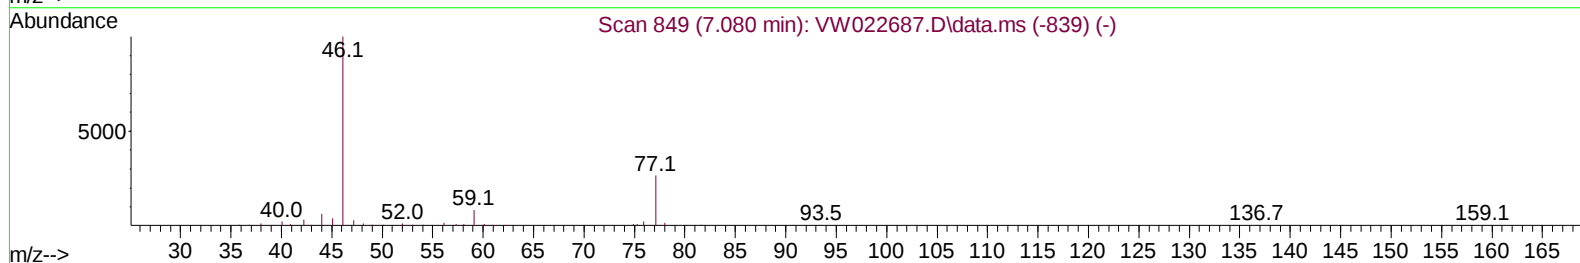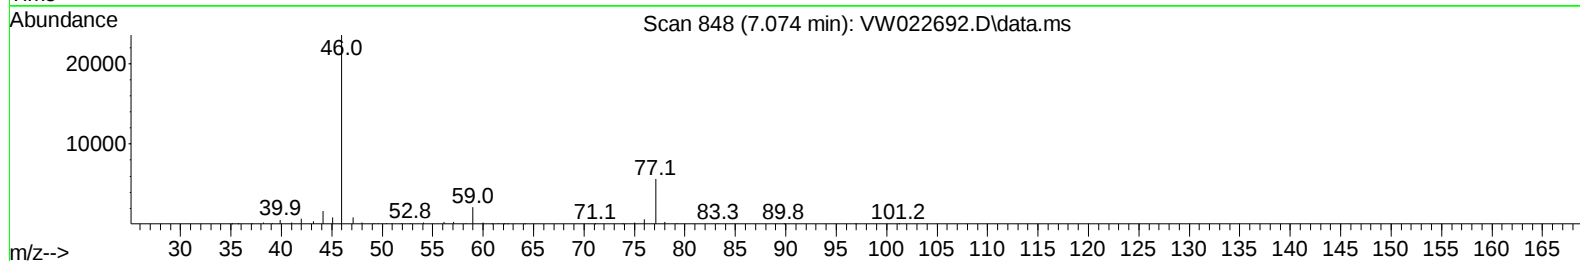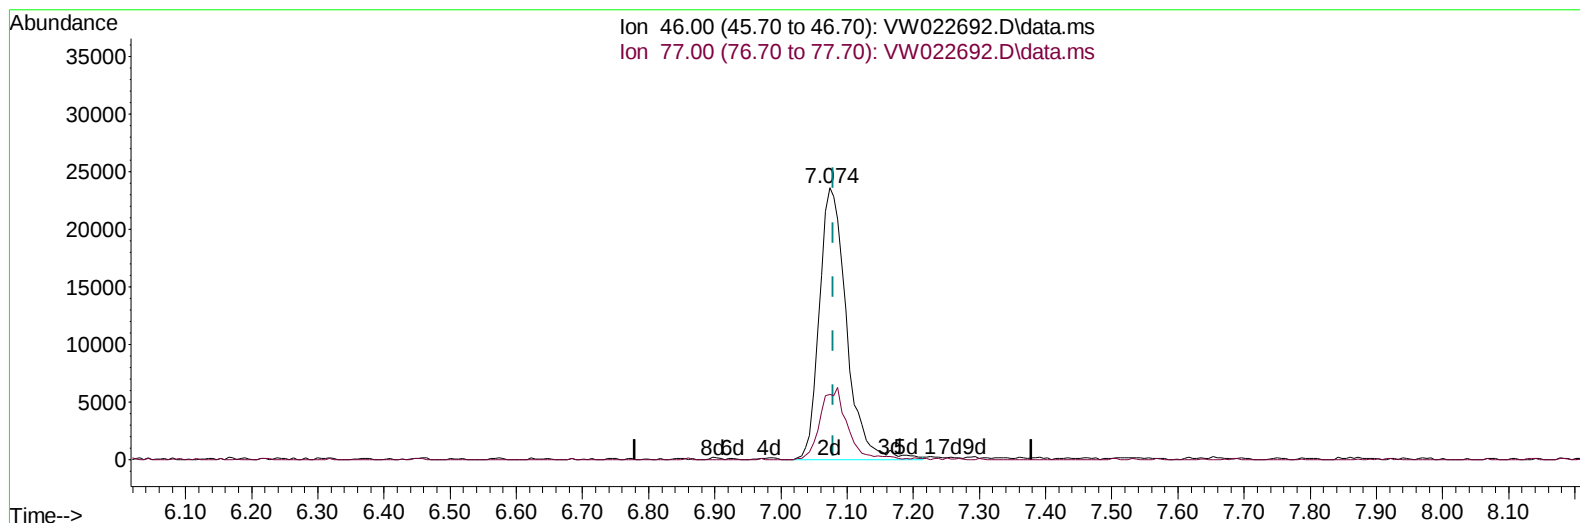

TIC: VW022692.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (-0.006) 55.15 ug/L m

response 67220

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	0.11#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022692.D
Acq On : 29 Apr 2022 11:57
Operator : SY/VA
Sample : N2603-11
Misc : 7.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW492

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

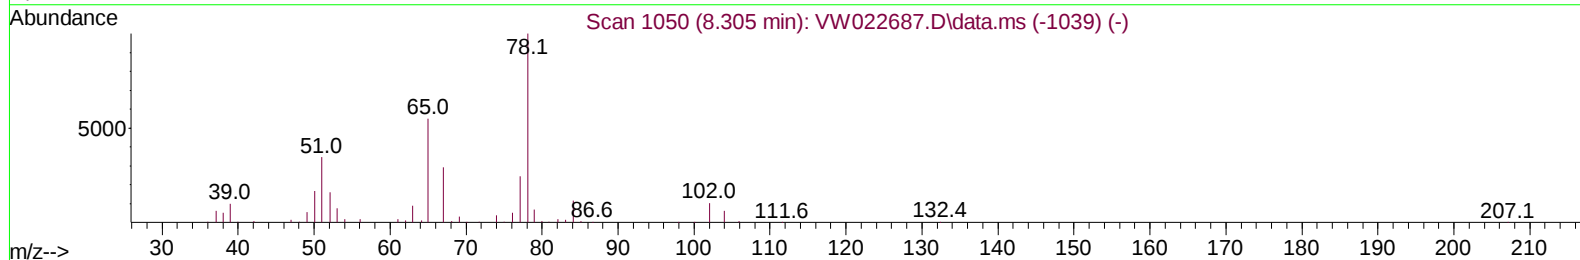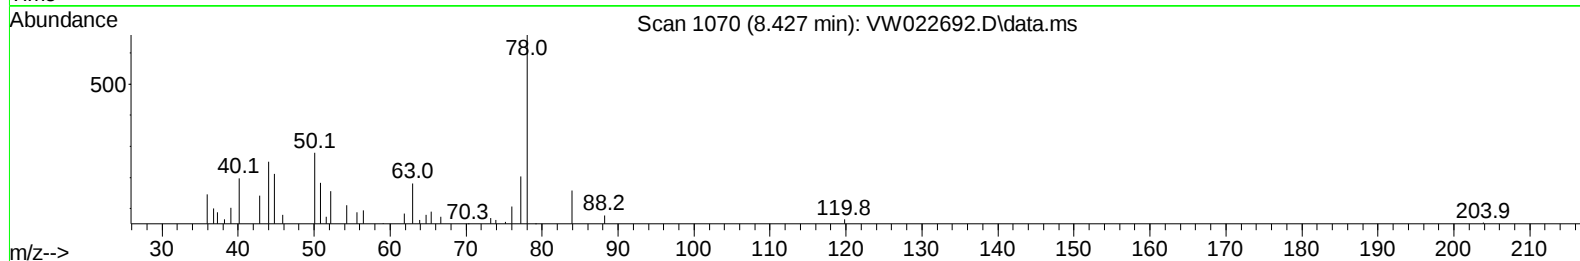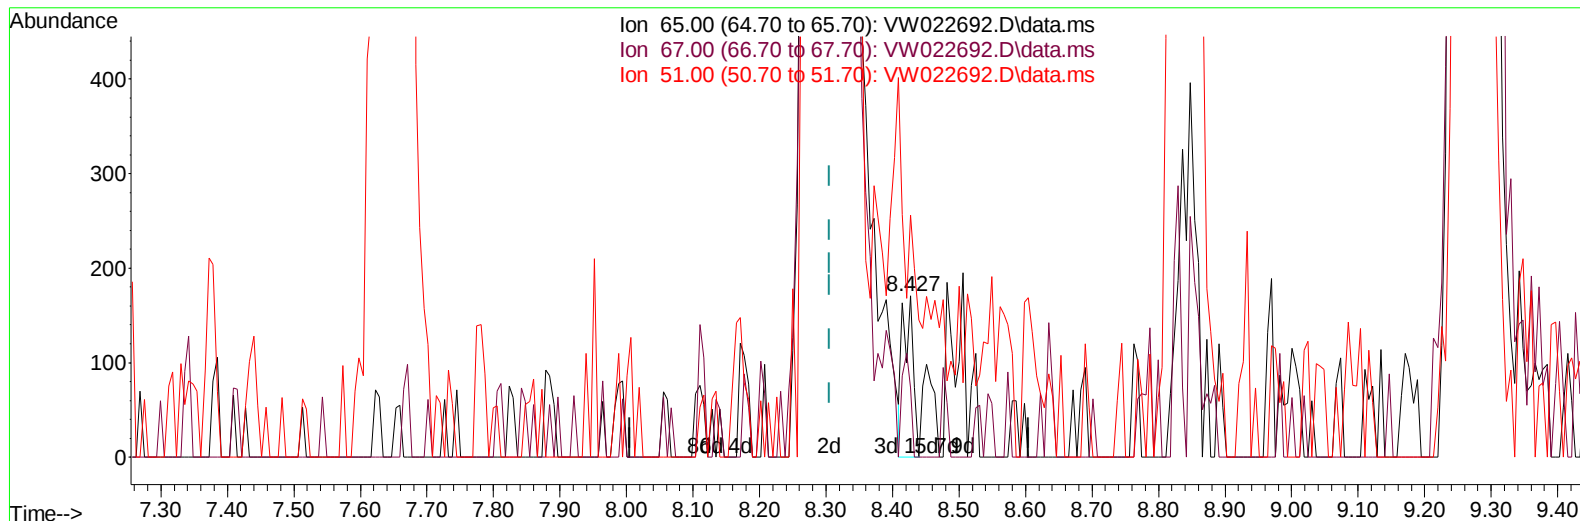

TIC: VW022692.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.427min (+ 0.122) 0.03 ug/L

response 186

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	52.69
51.00	99.30	84.95
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022692.D
 Acq On : 29 Apr 2022 11:57
 Operator : SY/VA
 Sample : N2603-11
 Misc : 7.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW492

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

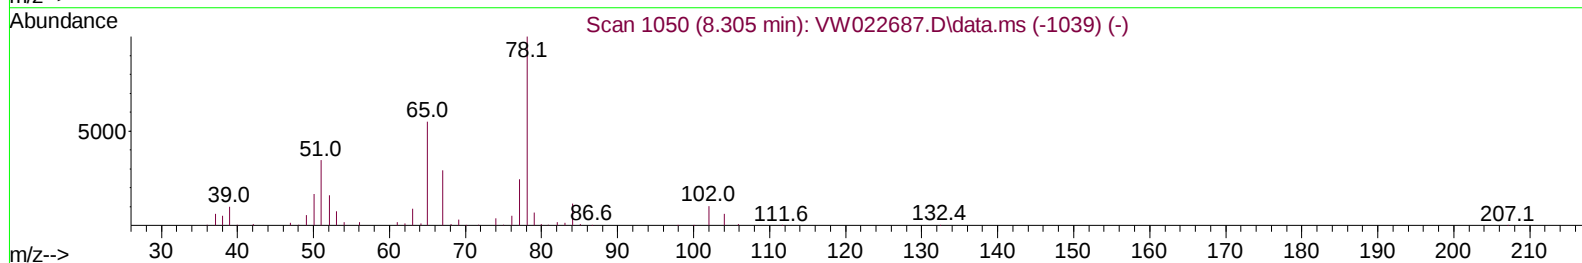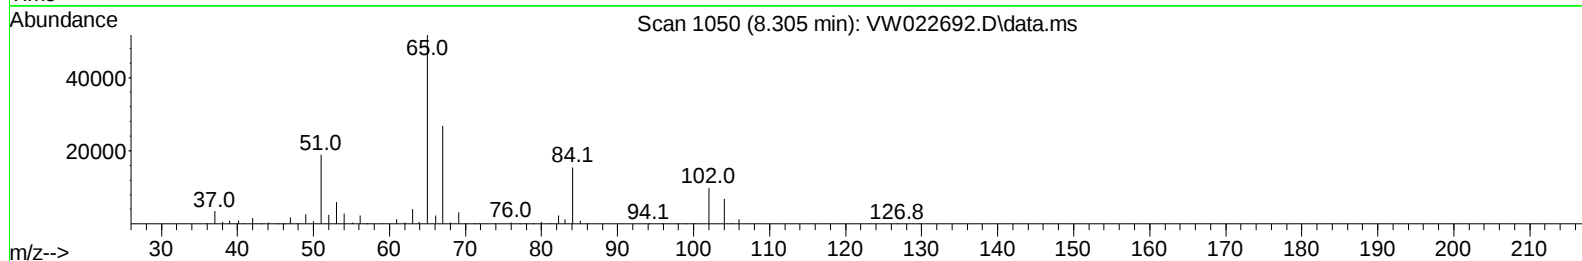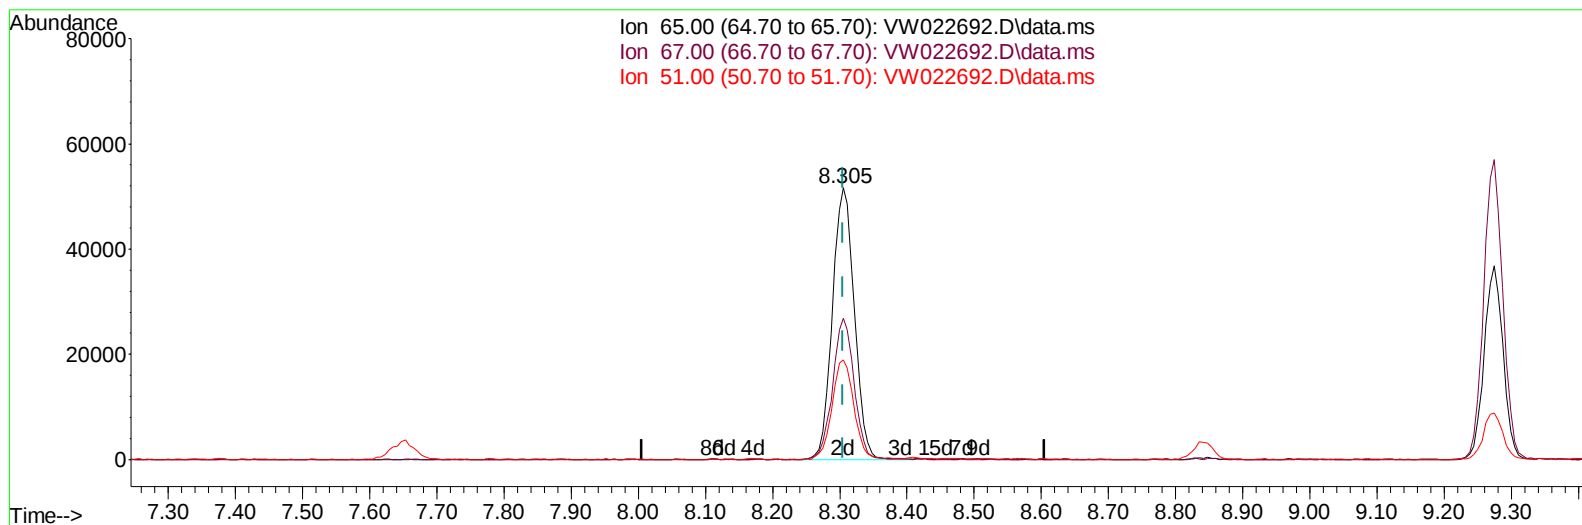

TIC: VW022692.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 20.72 ug/L m

response 116862

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.08#
51.00	99.30	0.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022692.D
 Acq On : 29 Apr 2022 11:57
 Operator : SY/VA
 Sample : N2603-11
 Misc : 7.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW492

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		315815	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		273301	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		95043	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		79833	11.435	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	45.720%		
7) Chloroethane-d5	2.885	69		70088	16.018	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.080%		
11) 1,1-Dichloroethene-d2	4.019	63		92574	10.223	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	40.880%#		
21) 2-Butanone-d5	7.074	46		67220m	55.147	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	110.300%		
24) Chloroform-d	7.647	84		201269	20.389	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	81.560%		
26) 1,2-Dichloroethane-d4	8.305	65		116862m	20.720	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	82.880%		
32) Benzene-d6	8.275	84		331345	19.844	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	79.360%		
36) 1,2-Dichloropropane-d6	9.275	67		112659	23.315	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	93.240%		
41) Toluene-d8	10.323	98		276039	16.879	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	67.520%		
43) trans-1,3-Dichloroprop...	10.579	79		38602	16.927	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	67.720%		
47) 2-Hexanone-d5	10.921	63		53225	59.203	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	118.400%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		116686	28.400	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	113.600%		
66) 1,2-Dichlorobenzene-d4	13.853	152		79366	23.576	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	94.320%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022692.D
Acq On : 29 Apr 2022 11:57
Operator : SY/VA
Sample : N2603-11
Misc : 7.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW492

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

