




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022693.D
Acq On : 29 Apr 2022 12:21
Operator : SY/VA
Sample : N2603-12RE
Misc : 6.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW493RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

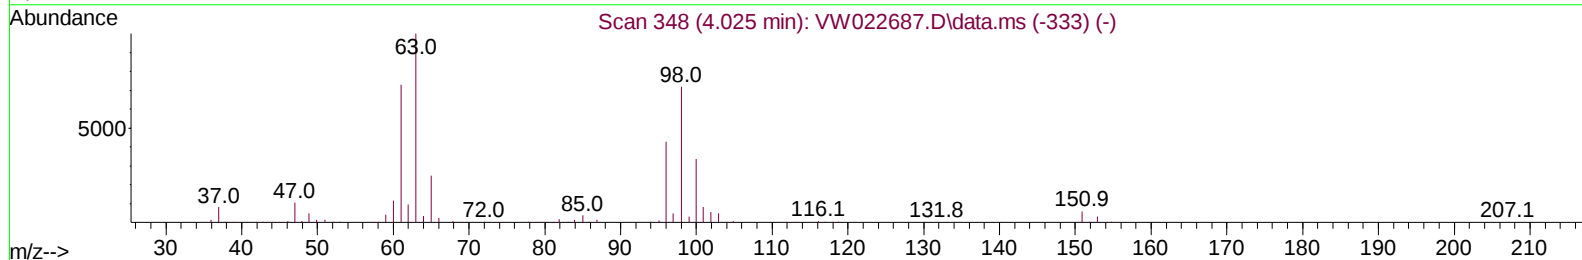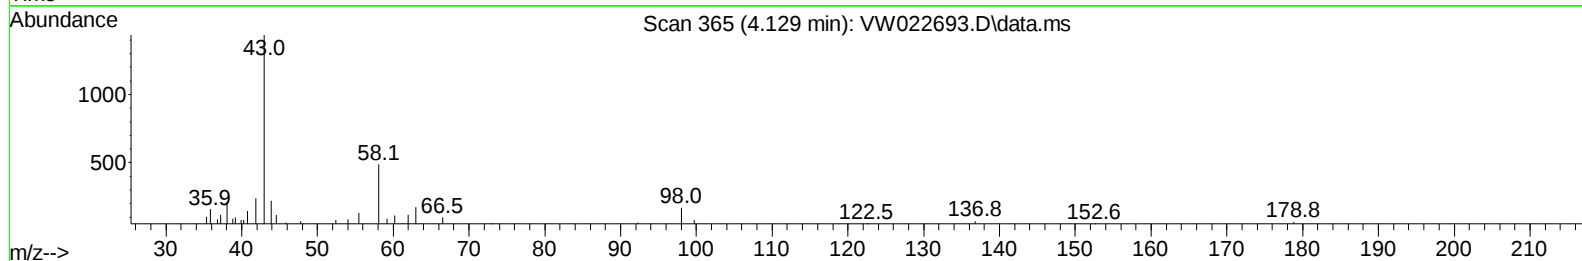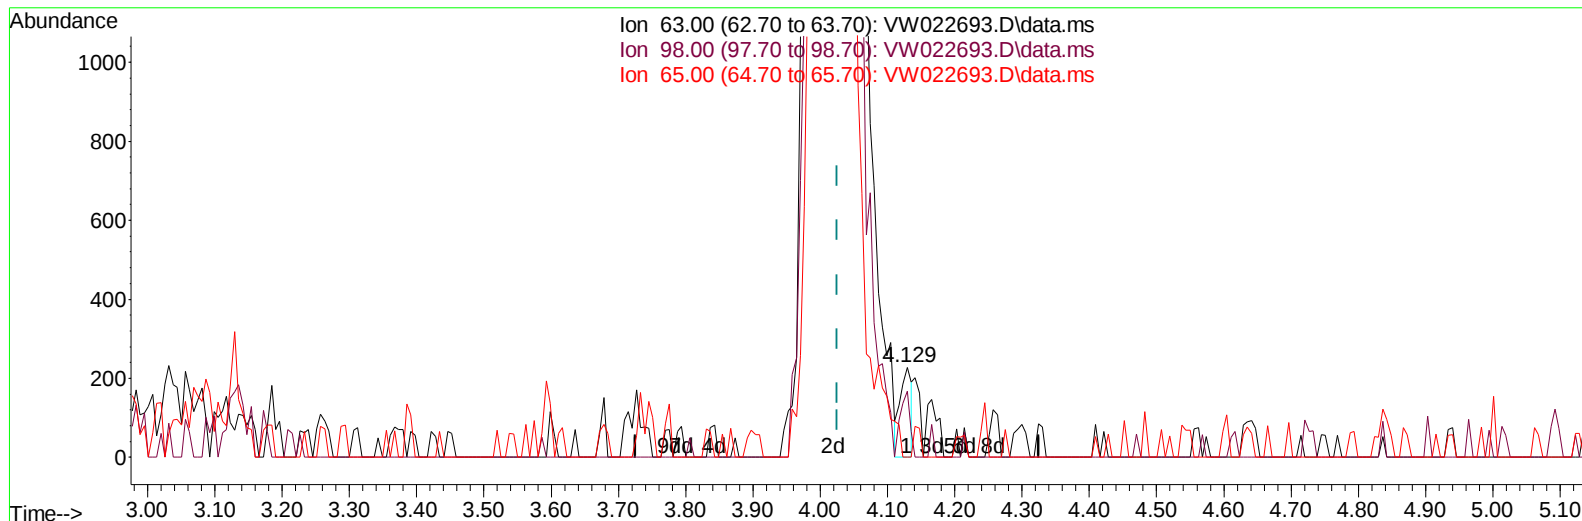

TIC: VW022693.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.129min (+ 0.104) 0.04 ug/L

response 269

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.50	63.20
65.00	22.80	20.45
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022693.D
 Acq On : 29 Apr 2022 12:21
 Operator : SY/VA
 Sample : N2603-12RE
 Misc : 6.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW493RE

Manual IntegrationsAPPROVED

Quant Time: Apr 29 22:24:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

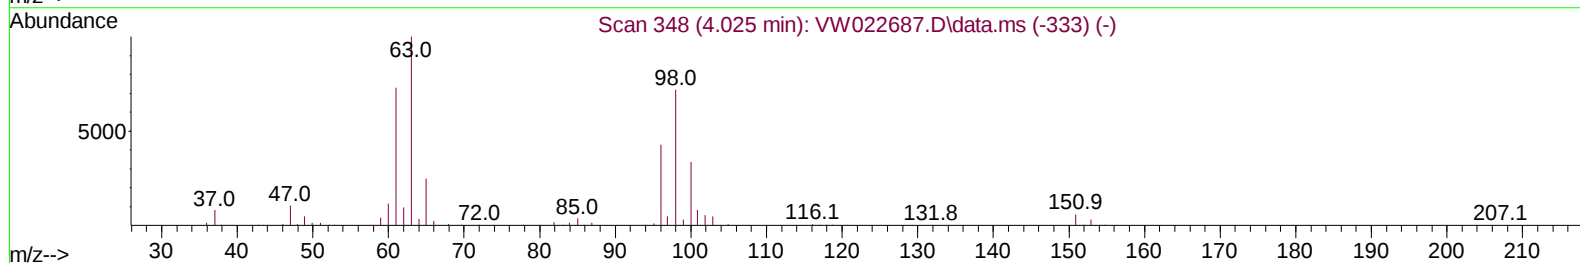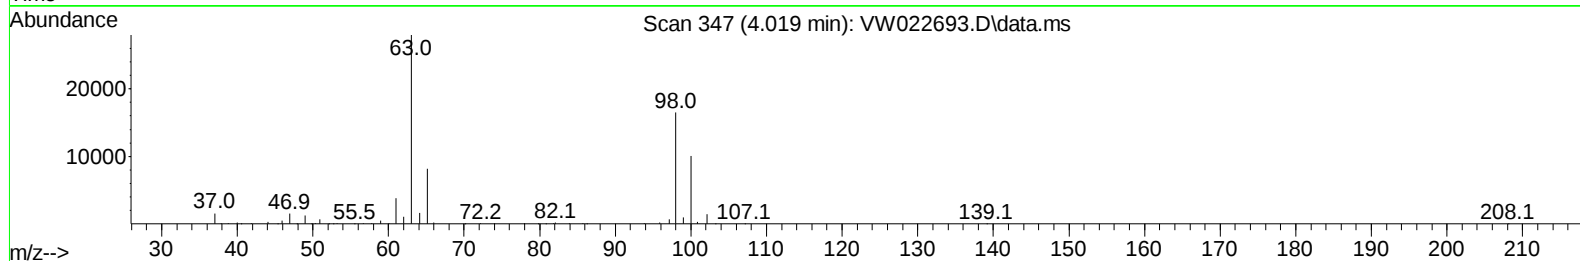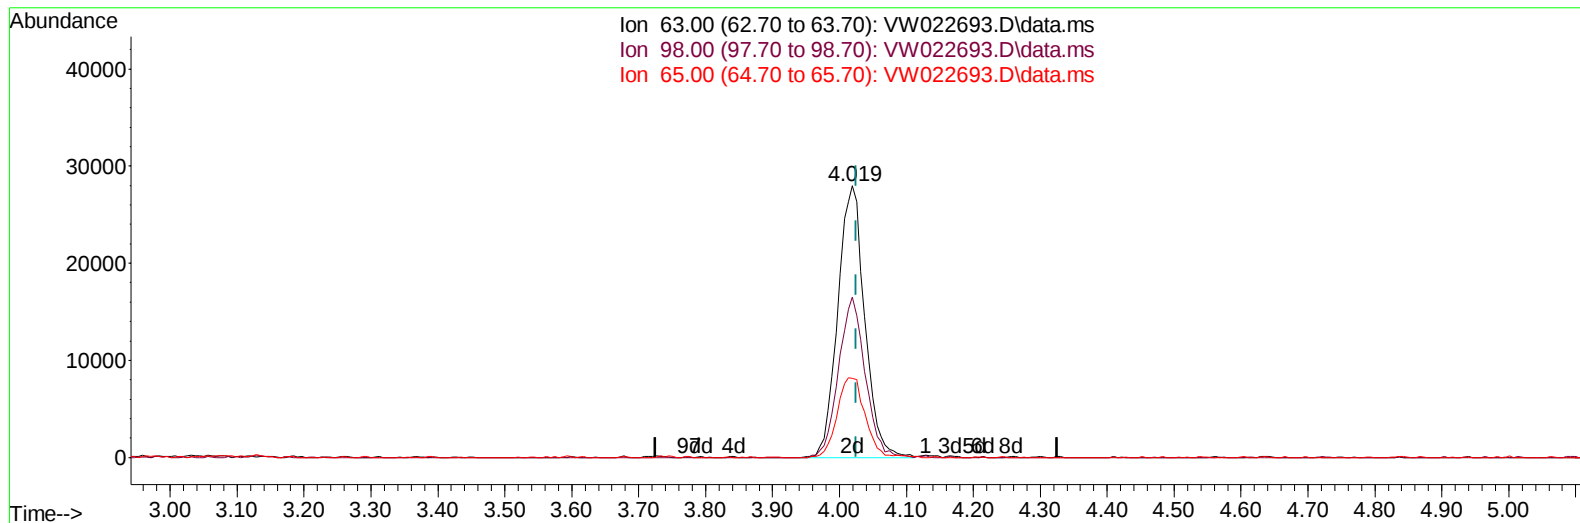

TIC: VW022693.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.006) 10.94 ug/L m

response 78021

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.50	0.22#
65.00	22.80	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022693.D
 Acq On : 29 Apr 2022 12:21
 Operator : SY/VA
 Sample : N2603-12RE
 Misc : 6.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW493RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		248703	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		151557	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		29555	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		74718	13.590	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.360%		
7) Chloroethane-d5	2.885	69		63648	18.471	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	73.880%		
11) 1,1-Dichloroethene-d2	4.019	63		78021m	10.941	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	43.760%#		
21) 2-Butanone-d5	7.074	46		73871	76.958	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	153.920%#		
24) Chloroform-d	7.647	84		173701	22.345	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	89.360%		
26) 1,2-Dichloroethane-d4	8.305	65		101346	22.818	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	91.280%		
32) Benzene-d6	8.275	84		277520	29.971	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	119.880%		
36) 1,2-Dichloropropane-d6	9.275	67		94858	35.400	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	141.600%#		
41) Toluene-d8	10.323	98		189291	20.873	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	83.480%		
43) trans-1,3-Dichloroprop...	10.579	79		25494	20.159	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	80.640%		
47) 2-Hexanone-d5	10.921	63		50075	100.442	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	200.880%#		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		97940	42.986	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	171.960%#		
66) 1,2-Dichlorobenzene-d4	13.853	152		31957	30.527	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	122.120%#		
Target Compounds							
13) Acetone	4.129	43		4159	6.364	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022693.D
Acq On : 29 Apr 2022 12:21
Operator : SY/VA
Sample : N2603-12RE
Misc : 6.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW493RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

