




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022694.D
 Acq On : 29 Apr 2022 12:45
 Operator : SY/VA
 Sample : N2603-06RE
 Misc : 8.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW487RE

Manual IntegrationsAPPROVED

Quant Time: Apr 29 22:24:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

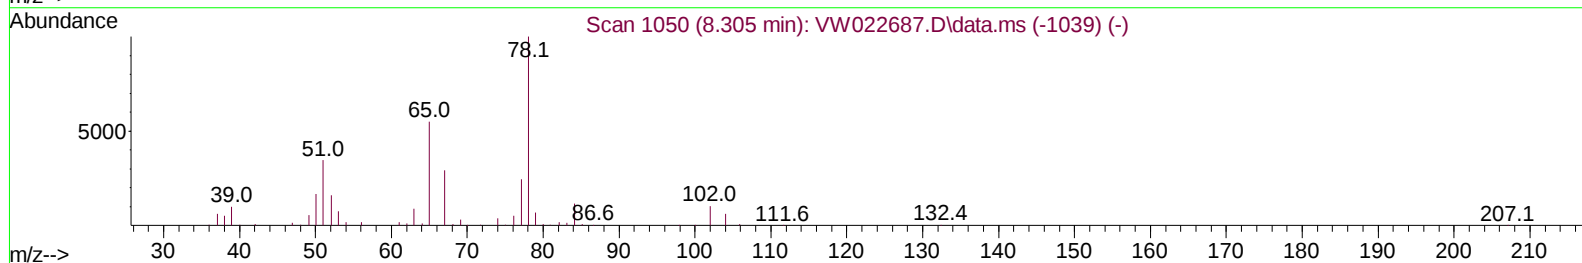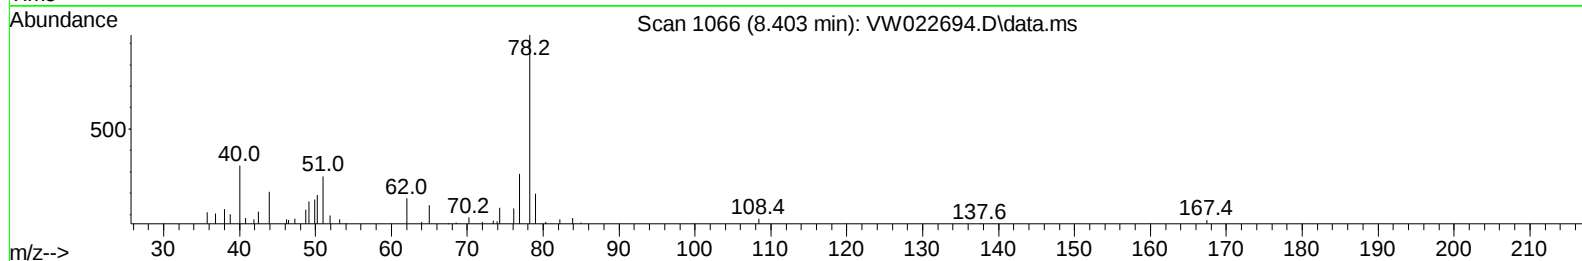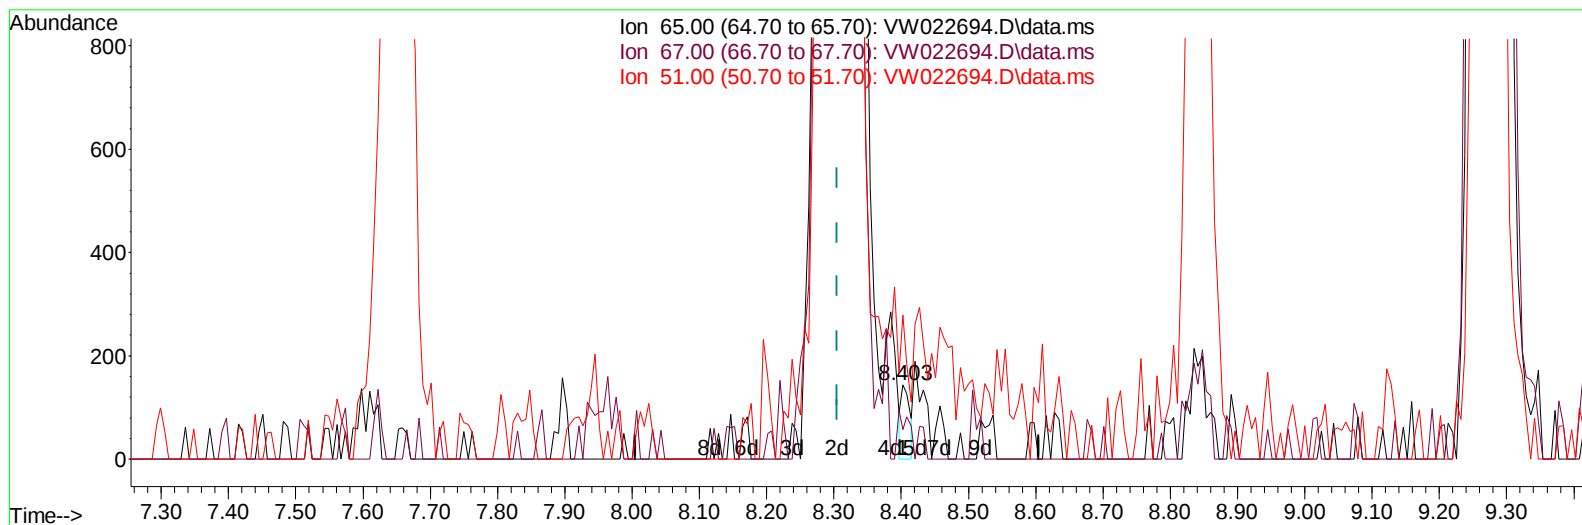

TIC: VW022694.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+ 0.097) 0.04 ug/L

response 128

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	42.97
51.00	99.30	124.22
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022694.D
 Acq On : 29 Apr 2022 12:45
 Operator : SY/VA
 Sample : N2603-06RE
 Misc : 8.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW487RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

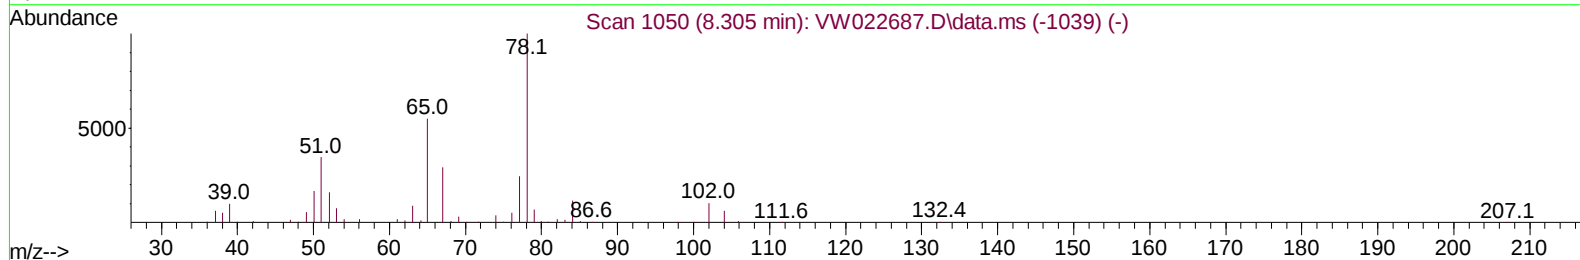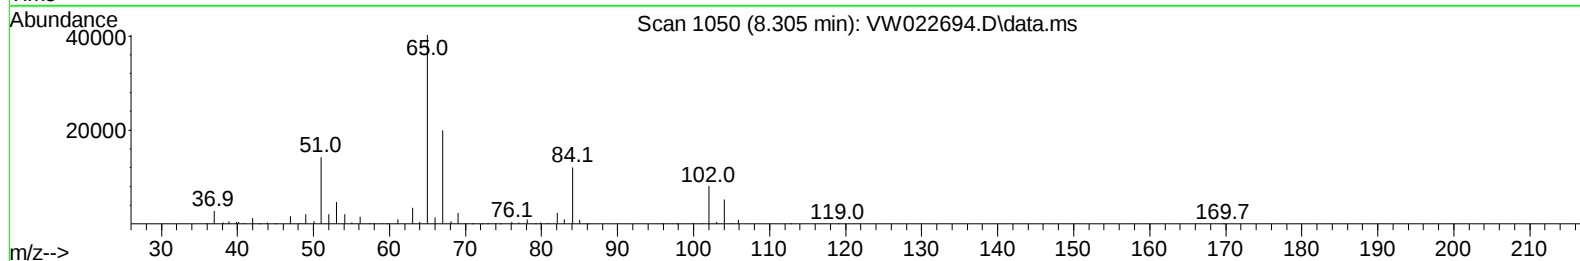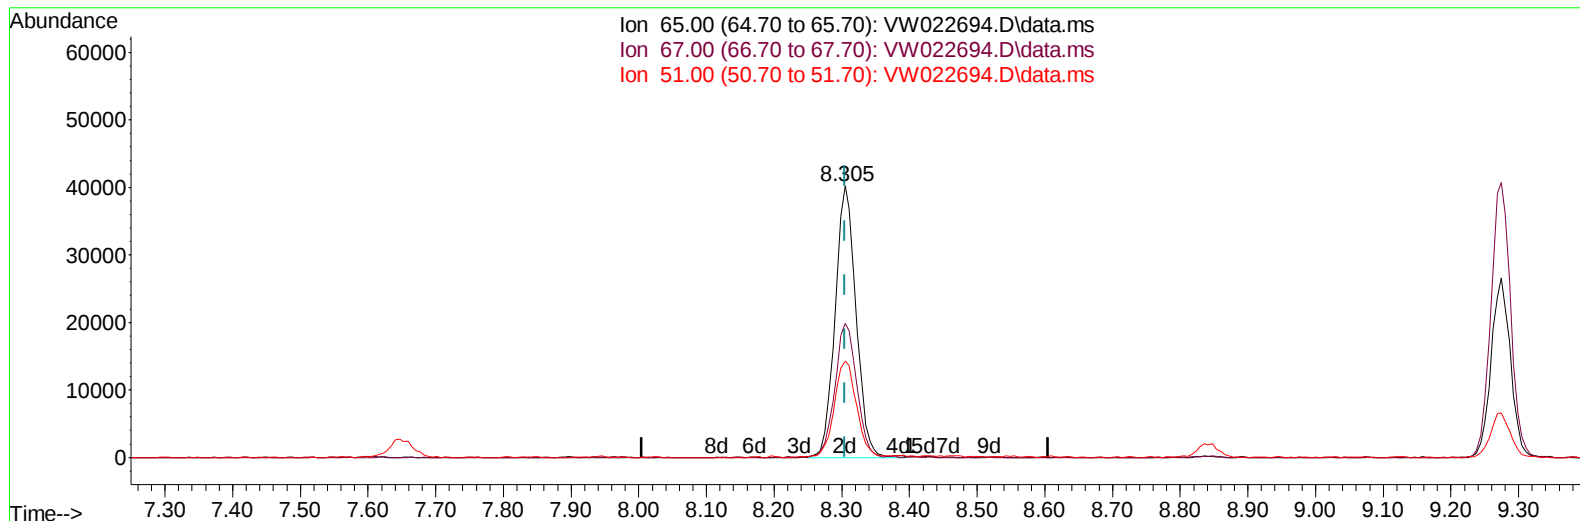

TIC: VW022694.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 26.19 ug/L m

response 86333

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.06#
51.00	99.30	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022694.D
 Acq On : 29 Apr 2022 12:45
 Operator : SY/VA
 Sample : N2603-06RE
 Misc : 8.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW487RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		184578	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		100427	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		18471	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		66266	16.240	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.960%		
7) Chloroethane-d5	2.885	69		53273	20.832	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	83.320%		
11) 1,1-Dichloroethene-d2	4.013	63		56585	10.692	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery =	42.760%#		
21) 2-Butanone-d5	7.080	46		64034	89.886	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	179.780%#		
24) Chloroform-d	7.647	84		149443	25.903	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	103.600%		
26) 1,2-Dichloroethane-d4	8.305	65		86333m	26.190	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	104.760%		
32) Benzene-d6	8.274	84		225911	36.819	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	147.280%#		
36) 1,2-Dichloropropane-d6	9.274	67		82755	46.607	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	186.440%#		
41) Toluene-d8	10.323	98		134690	22.414	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	89.640%		
43) trans-1,3-Dichloroprop...	10.579	79		18318	21.860	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	87.440%		
47) 2-Hexanone-d5	10.920	63		42191	127.714	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	255.420%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		84643	56.064	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	224.240%#		
66) 1,2-Dichlorobenzene-d4	13.853	152		22229	33.977	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	135.920%#		
Target Compounds							Qvalue
13) Acetone	4.129	43		4798	9.892	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022694.D
Acq On : 29 Apr 2022 12:45
Operator : SY/VA
Sample : N2603-06RE
Misc : 8.44g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW487RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

