




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022695.D
 Acq On : 29 Apr 2022 13:09
 Operator : SY/VA
 Sample : N2603-13RE
 Misc : 7.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW494RE

Manual IntegrationsAPPROVED

Quant Time: Apr 29 22:24:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

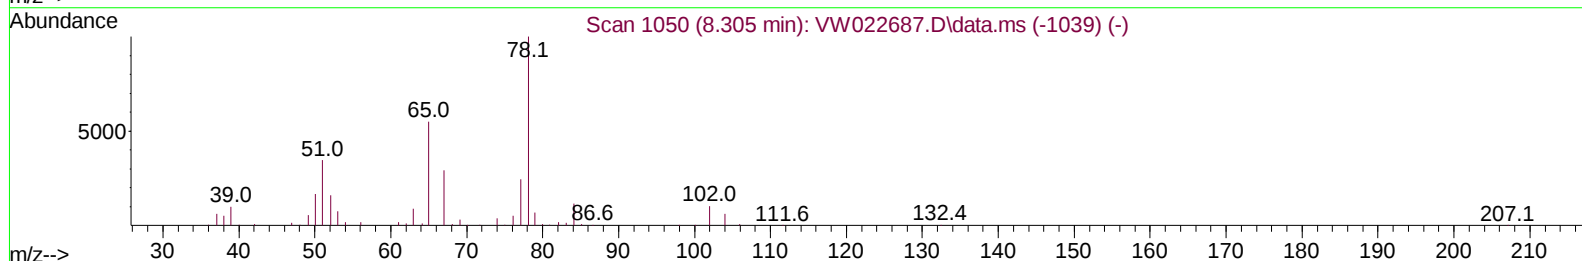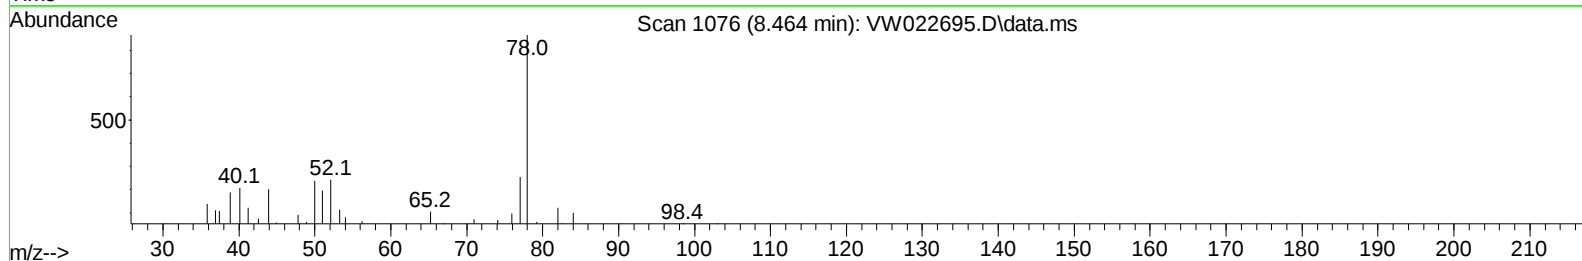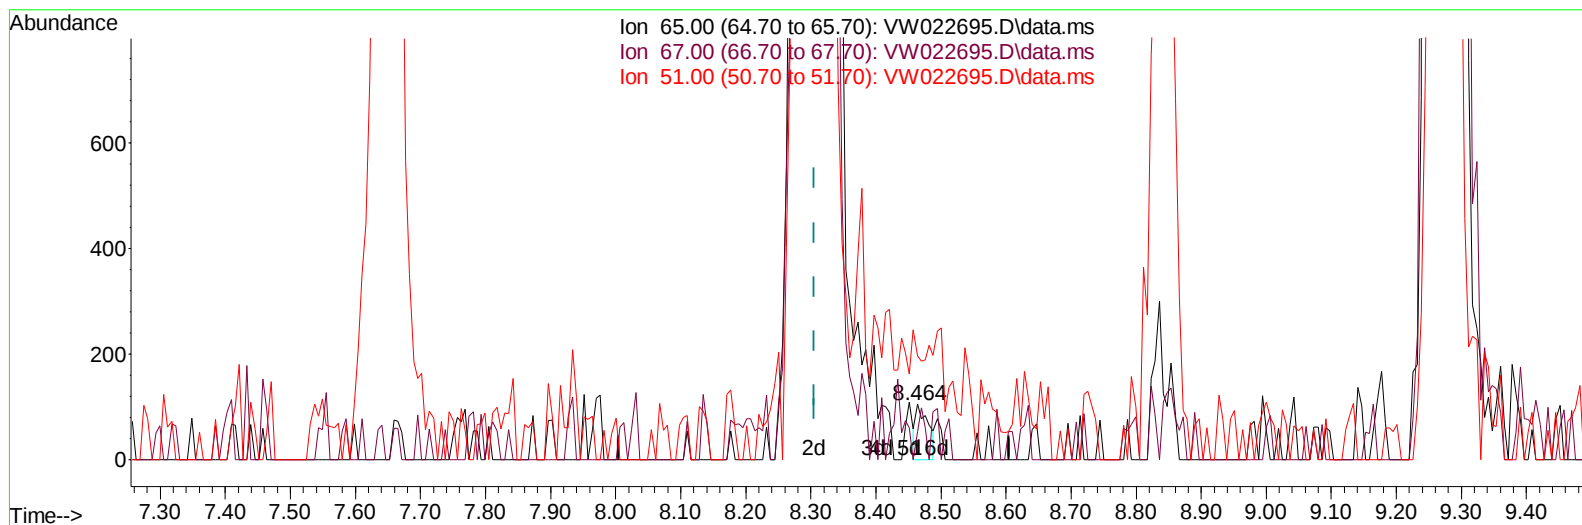

TIC: VW022695.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.464min (+ 0.159) 0.05 ug/L

response 141

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	54.61
51.00	99.30	104.96
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022695.D
Acq On : 29 Apr 2022 13:09
Operator : SY/VA
Sample : N2603-13RE
Misc : 7.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW494RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

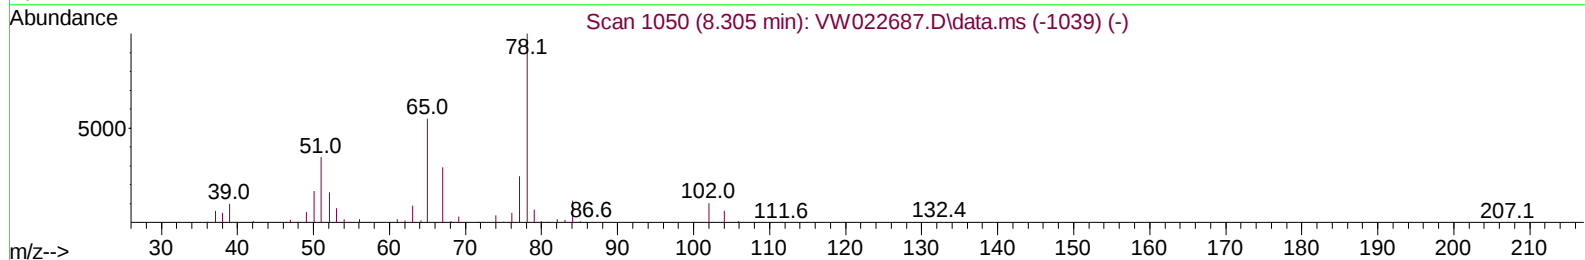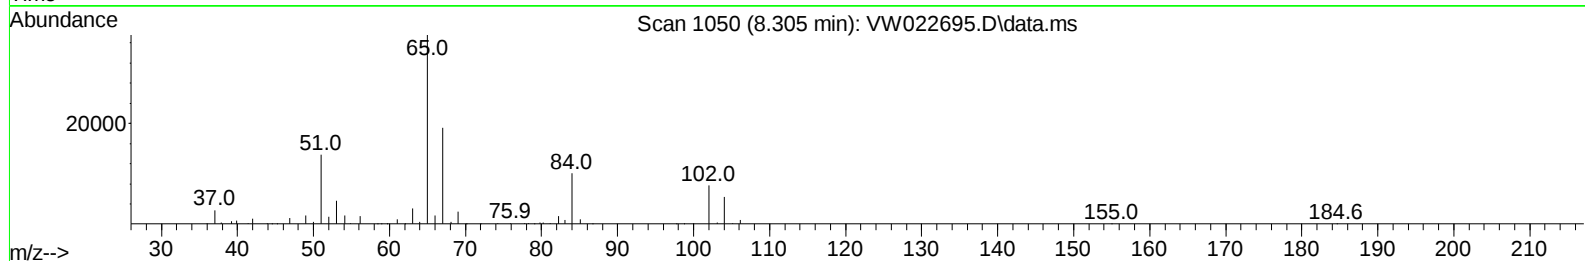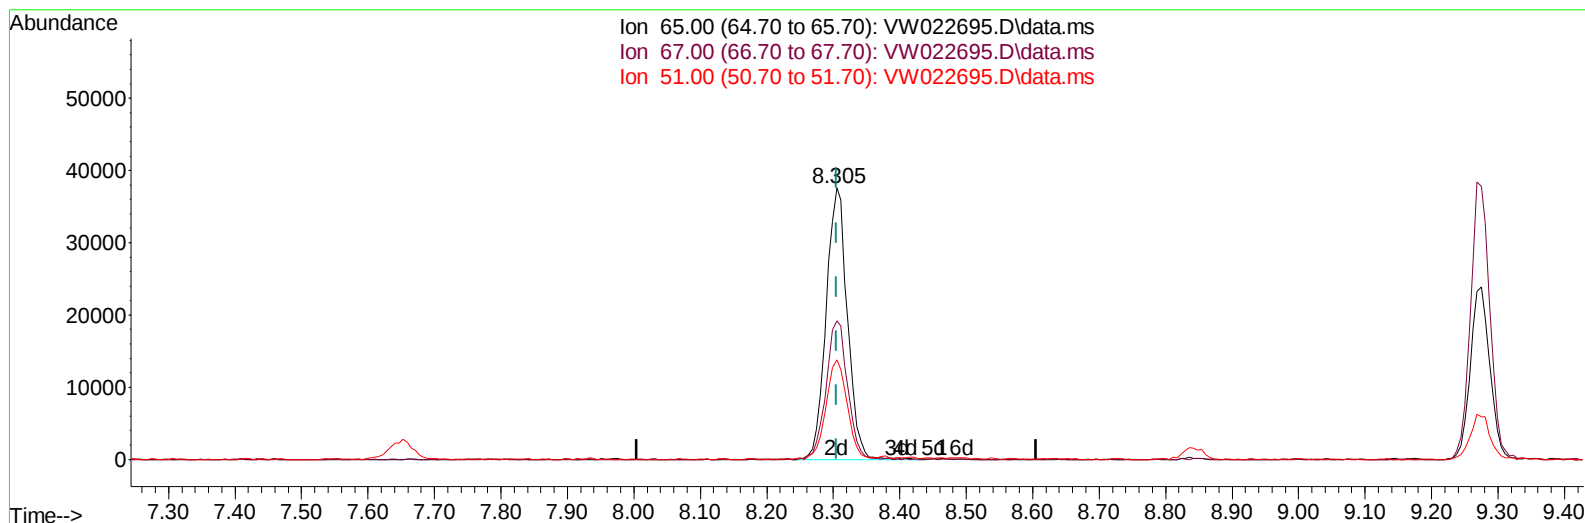

TIC: VW022695.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 29.14 ug/L m

response 83453

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.09#
51.00	99.30	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022695.D
 Acq On : 29 Apr 2022 13:09
 Operator : SY/VA
 Sample : N2603-13RE
 Misc : 7.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW494RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	160385	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	69639	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	10446	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	71561	20.183	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.720%	
7) Chloroethane-d5	2.885	69	60158	27.072	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	108.280%	
11) 1,1-Dichloroethene-d2	4.019	63	60518	13.160	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	52.640%	
21) 2-Butanone-d5	7.080	46	67660	109.302	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	218.600%#	
24) Chloroform-d	7.647	84	143114	28.548	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	114.200%	
26) 1,2-Dichloroethane-d4	8.305	65	83453m	29.136	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	116.560%	
32) Benzene-d6	8.275	84	209127	49.152	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	196.600%#	
36) 1,2-Dichloropropane-d6	9.268	67	77238	62.731	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	250.920%#	
41) Toluene-d8	10.323	98	108811	26.113	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	104.440%	
43) trans-1,3-Dichloroprop...	10.579	79	13973	24.047	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	96.200%	
47) 2-Hexanone-d5	10.921	63	38720	169.025	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	338.060%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	73781	70.475	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	281.880%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	11867	32.073	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	128.280%#	
Target Compounds						
13) Acetone	4.129	43	3877	9.199	ug/L	73
14) Carbon disulfide	4.379	76	6771	0.953	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022695.D
Acq On : 29 Apr 2022 13:09
Operator : SY/VA
Sample : N2603-13RE
Misc : 7.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW494RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

