




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022696.D
Acq On : 29 Apr 2022 13:33
Operator : SY/VA
Sample : VIBLK439
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK439

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

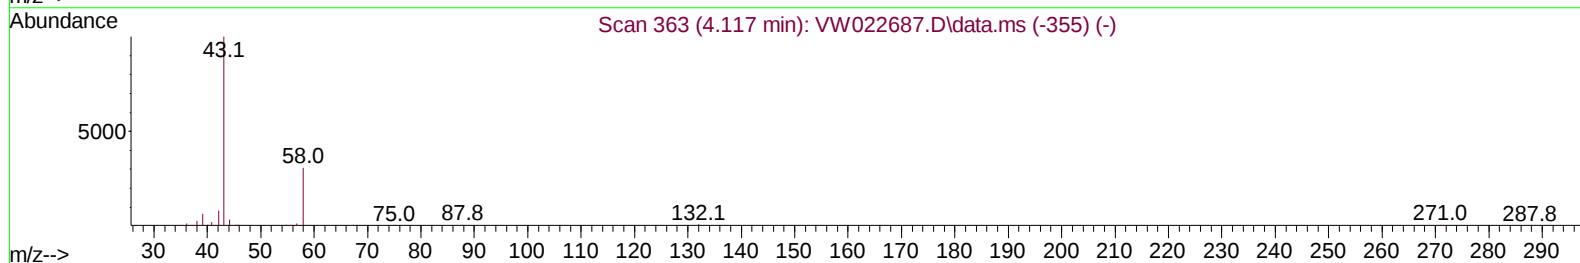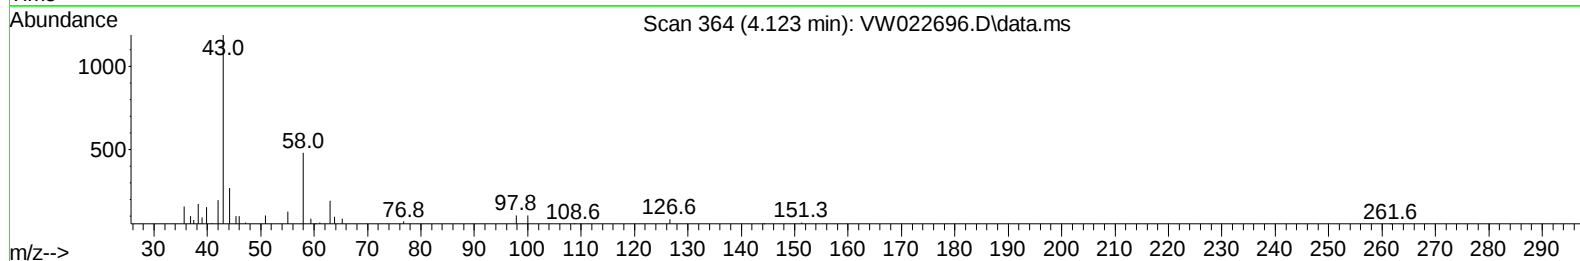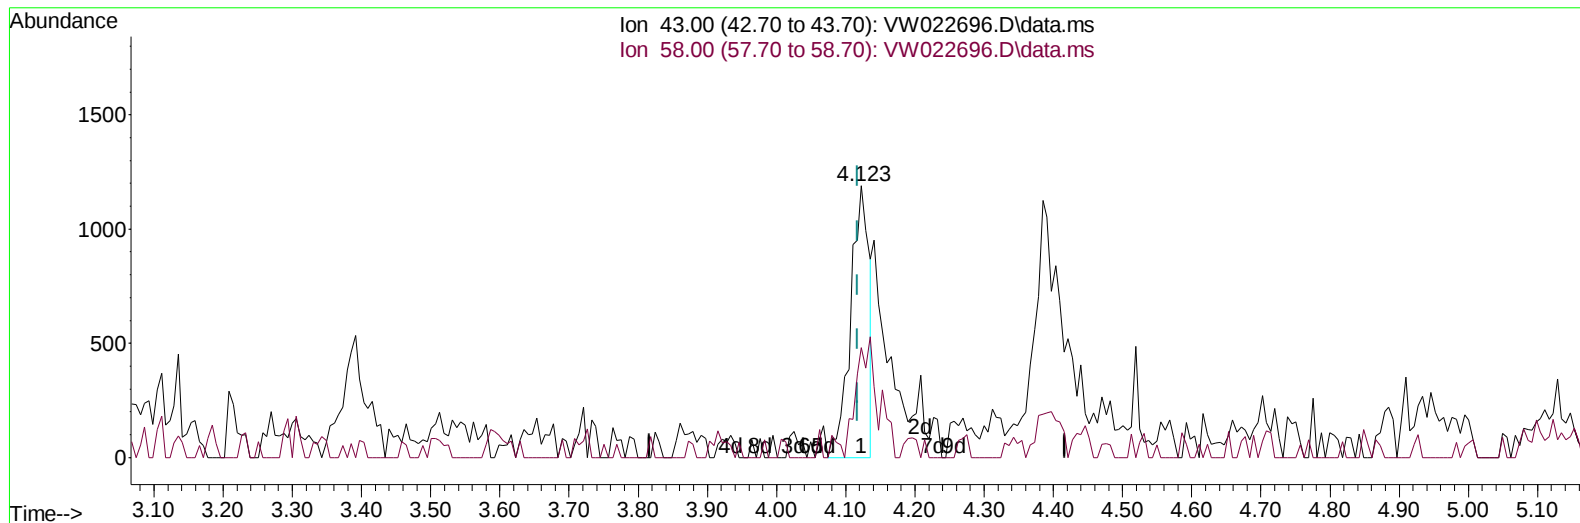

TIC: VW022696.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 3.16 ug/L

response 2202

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	26.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022696.D
 Acq On : 29 Apr 2022 13:33
 Operator : SY/VA
 Sample : VIBLK439
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK439

Manual IntegrationsAPPROVED

Quant Time: Apr 29 22:24:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

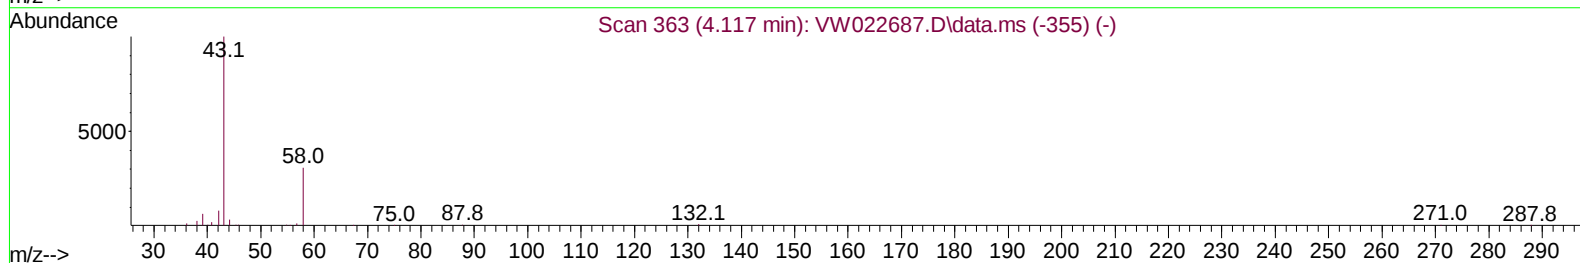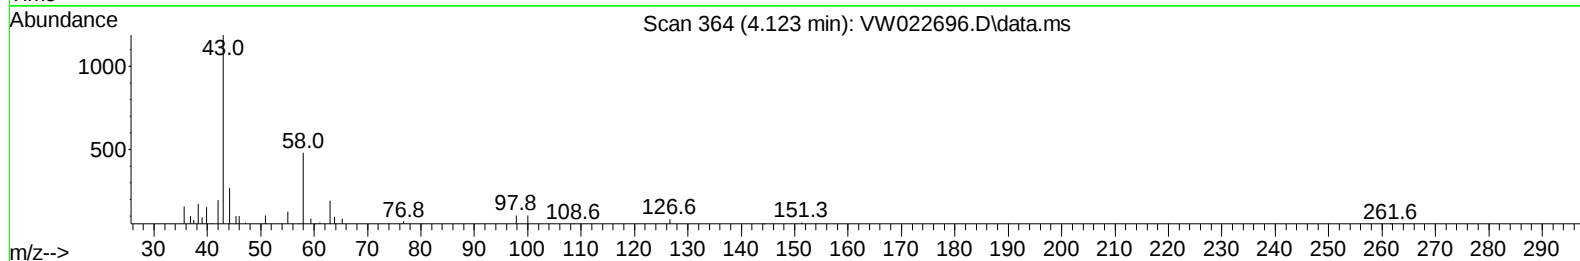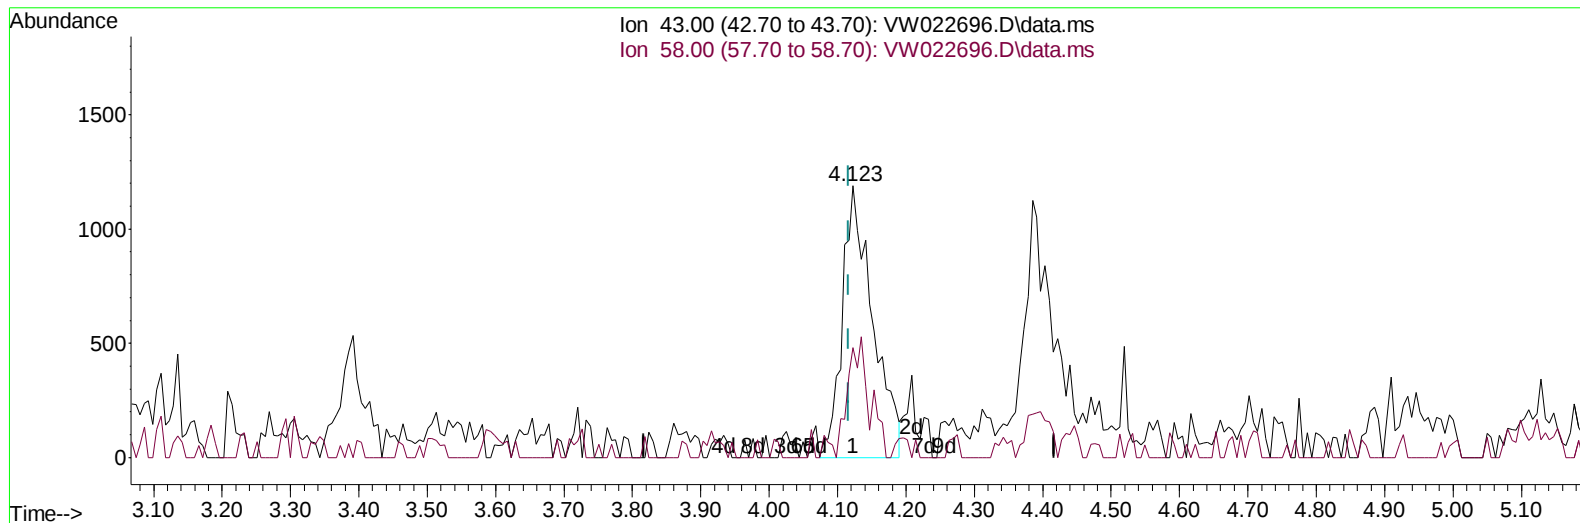

TIC: VW022696.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 5.26 ug/L m

response 3666

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	15.74
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022696.D
 Acq On : 29 Apr 2022 13:33
 Operator : SY/VA
 Sample : VIBLK439
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK439

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		265077	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		262701	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		129625	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		120136	20.501	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	82.000%	
7) Chloroethane-d5	2.885	69		85874	23.382	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.520%	
11) 1,1-Dichloroethene-d2	4.019	63		131454	17.295	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	69.200%	
21) 2-Butanone-d5	7.073	46		65447	63.970	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	127.940%	
24) Chloroform-d	7.646	84		213310	25.745	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	103.000%	
26) 1,2-Dichloroethane-d4	8.305	65		121381	25.640	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	102.560%	
32) Benzene-d6	8.274	84		412051	25.673	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	102.680%	
36) 1,2-Dichloropropane-d6	9.274	67		121708	26.204	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	104.800%	
41) Toluene-d8	10.323	98		390538	24.845	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	99.360%	
43) trans-1,3-Dichloroprop...	10.579	79		47805	21.809	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	87.240%	
47) 2-Hexanone-d5	10.926	63		51580	59.688	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	119.380%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		114182	28.912	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	115.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152		130171	28.351	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	113.400%	
Target Compounds							
13) Acetone	4.123	43		3666m	5.263	ug/L	
16) Methylene chloride	4.921	84		16302	4.087	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022696.D
Acq On : 29 Apr 2022 13:33
Operator : SY/VA
Sample : VIBLK439
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK439

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

