




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022710.D
 Acq On : 29 Apr 2022 20:28
 Operator : SY/VA
 Sample : N2603-19
 Misc : 7.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A0

Manual IntegrationsAPPROVED

Quant Time: Apr 30 02:00:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

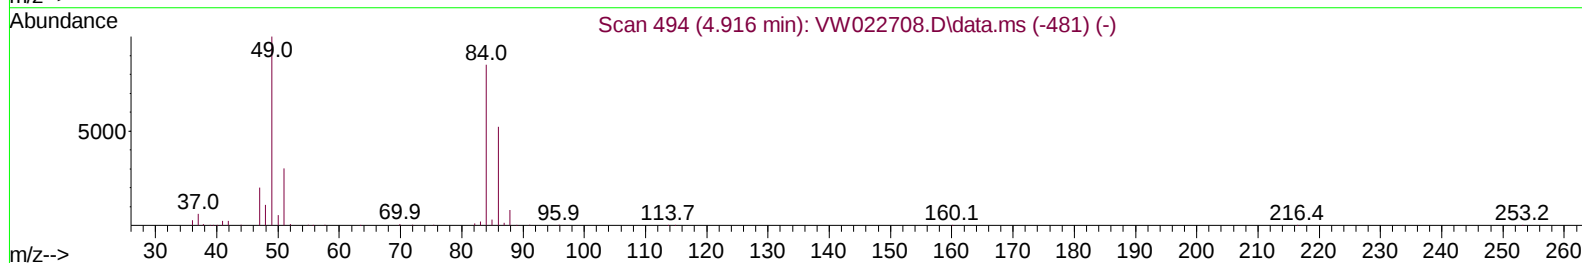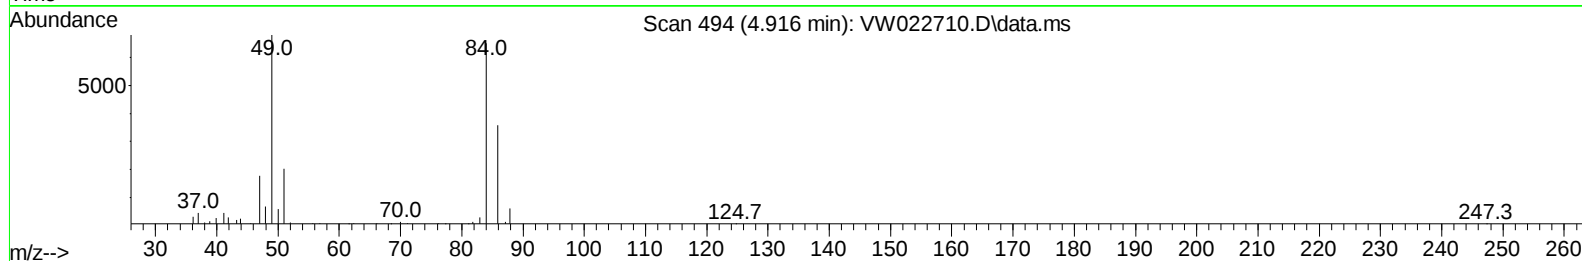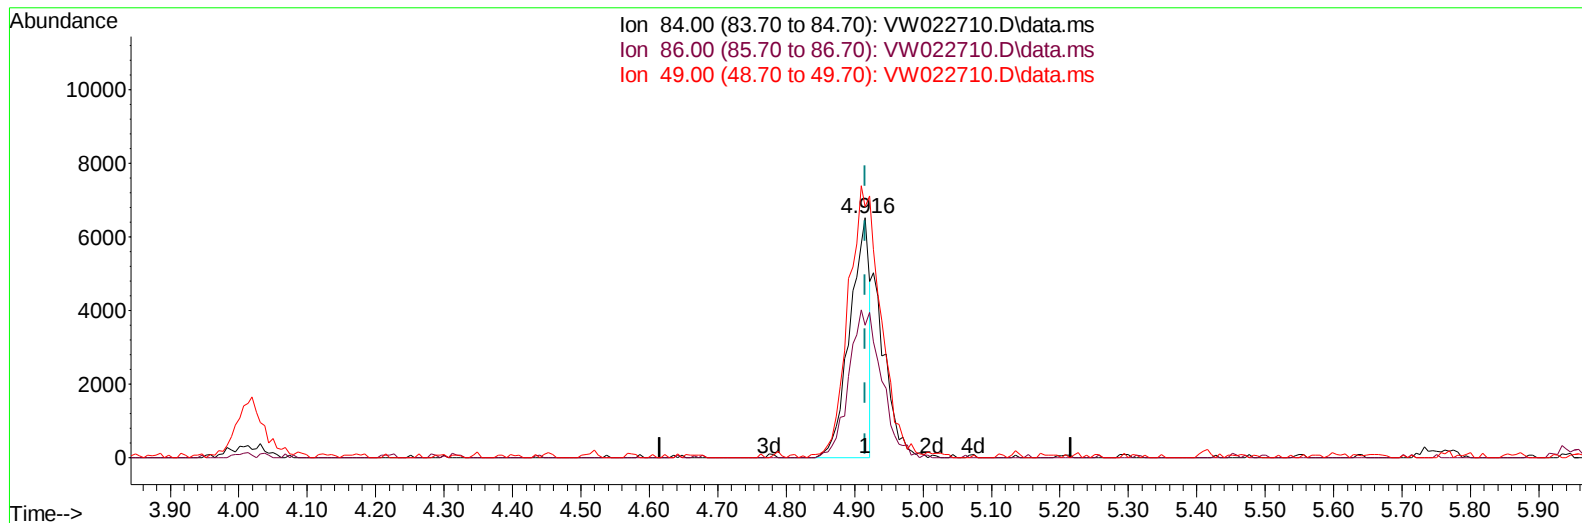

TIC: VW022710.D\data.ms

(16) Methylene chloride (T)

4.916min (0.000) 3.33 ug/L

response 12936

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.10	55.13
49.00	134.60	104.64
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022710.D
 Acq On : 29 Apr 2022 20:28
 Operator : SY/VA
 Sample : N2603-19
 Misc : 7.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A0

Manual IntegrationsAPPROVED

Quant Time: Apr 30 02:00:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

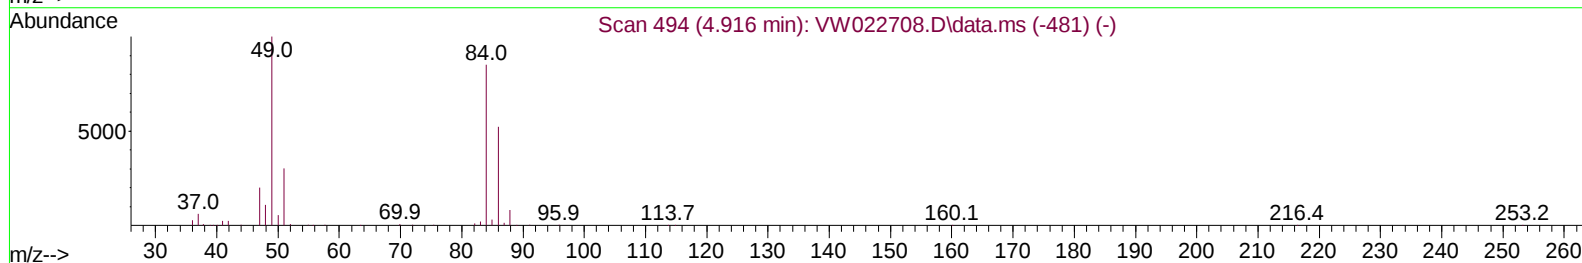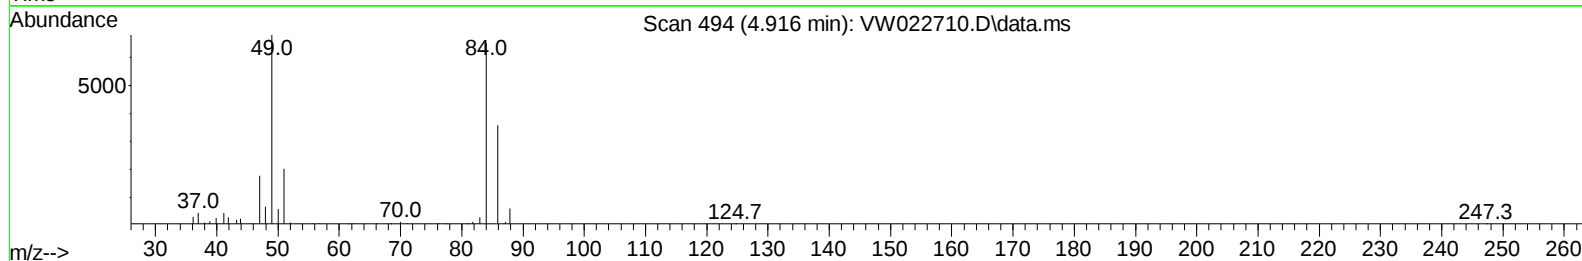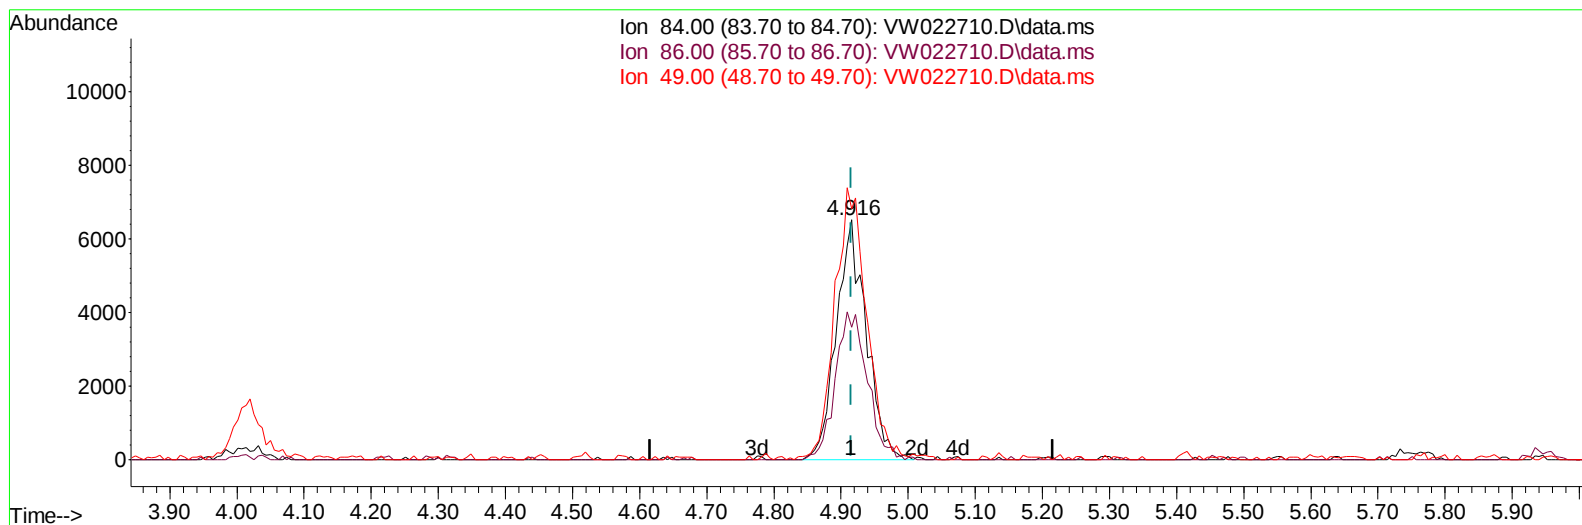

TIC: VW022710.D\data.ms

(16) Methylene chloride (T)

4.916min (0.000) 5.16 ug/L m

response 20034

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.10	55.13
49.00	134.60	104.64
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022710.D
 Acq On : 29 Apr 2022 20:28
 Operator : SY/VA
 Sample : N2603-19
 Misc : 7.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 30 02:00:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		258201	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		257134	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		128048	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		118675	20.791	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.160%	
7) Chloroethane-d5	2.886	69		83736	23.407	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.640%	
11) 1,1-Dichloroethene-d2	4.013	63		121550	16.418	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	65.680%	
21) 2-Butanone-d5	7.098	46		44590	44.744	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135		Recovery	=	89.480%	
24) Chloroform-d	7.647	84		196825	24.388	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	97.560%	
26) 1,2-Dichloroethane-d4	8.305	65		107389	23.289	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	93.160%	
32) Benzene-d6	8.275	84		386247	24.586	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	98.360%	
36) 1,2-Dichloropropane-d6	9.275	67		110311	24.264	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	97.040%	
41) Toluene-d8	10.323	98		358528	23.302	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	93.200%	
43) trans-1,3-Dichloroprop...	10.579	79		42031	19.590	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	78.360%	
47) 2-Hexanone-d5	10.927	63		36570	43.235	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	86.460%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		92278	23.871	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	95.480%	
66) 1,2-Dichlorobenzene-d4	13.853	152		120296	26.523	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	106.080%	
Target Compounds							
16) Methylene chloride	4.916	84		20034m	5.156	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022710.D
Acq On : 29 Apr 2022 20:28
Operator : SY/VA
Sample : N2603-19
Misc : 7.03g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4A0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 30 02:00:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 30 01:41:13 2022
Response via : Initial Calibration

