




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022712.D
 Acq On : 29 Apr 2022 21:41
 Operator : SY/VA
 Sample : N2638-01
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXKZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 30 02:00:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/04/2022

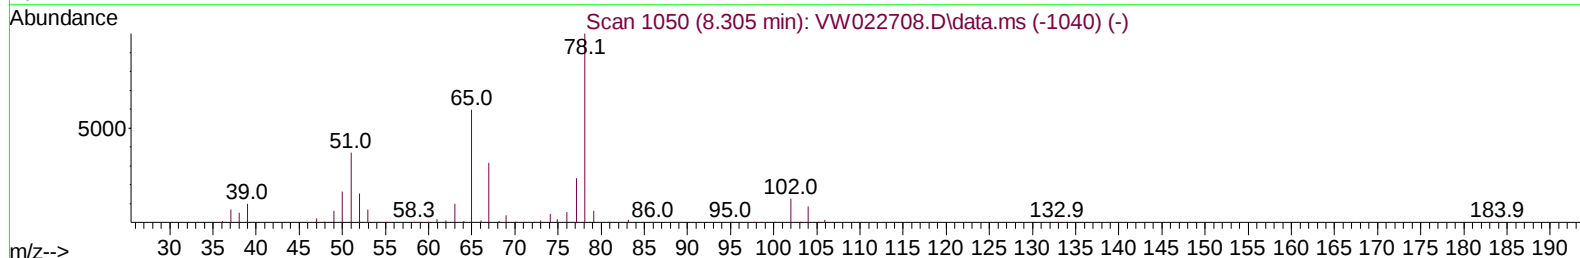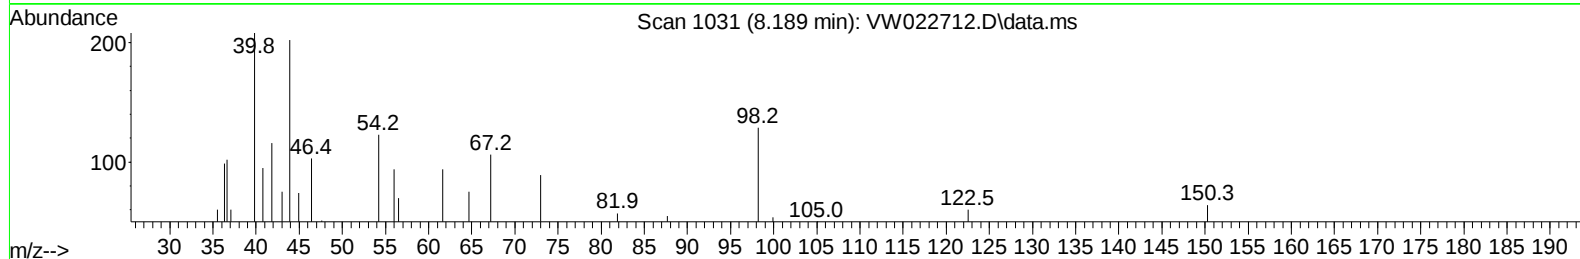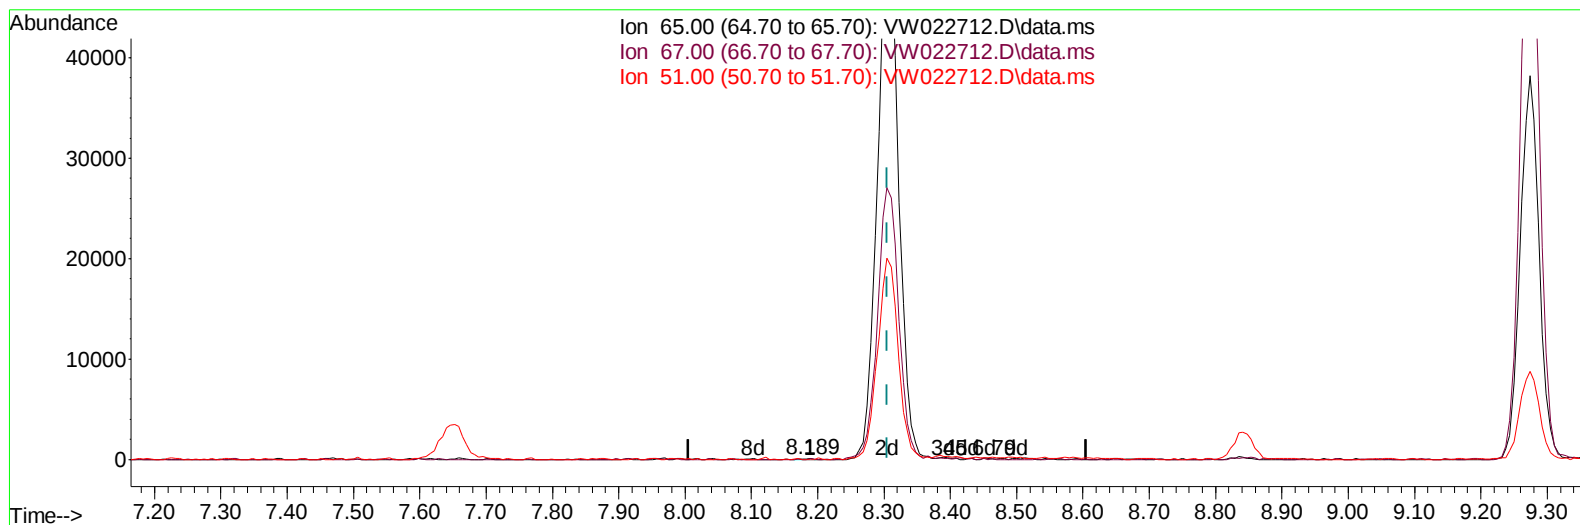

TIC: VW022712.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.189min (-0.116) 0.02 ug/L

response 95

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	62.11
51.00	99.30	76.84
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022712.D
Acq On : 29 Apr 2022 21:41
Operator : SY/VA
Sample : N2638-01
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXKZ2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/04/2022
Supervised By :Semsettin Yesilyurt 05/04/2022

Quant Time: Apr 30 02:00:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 30 01:41:13 2022
Response via : Initial Calibration

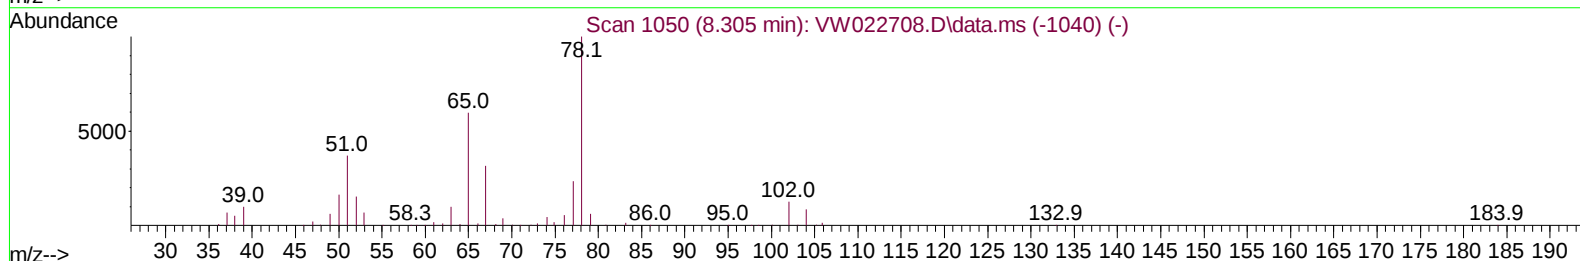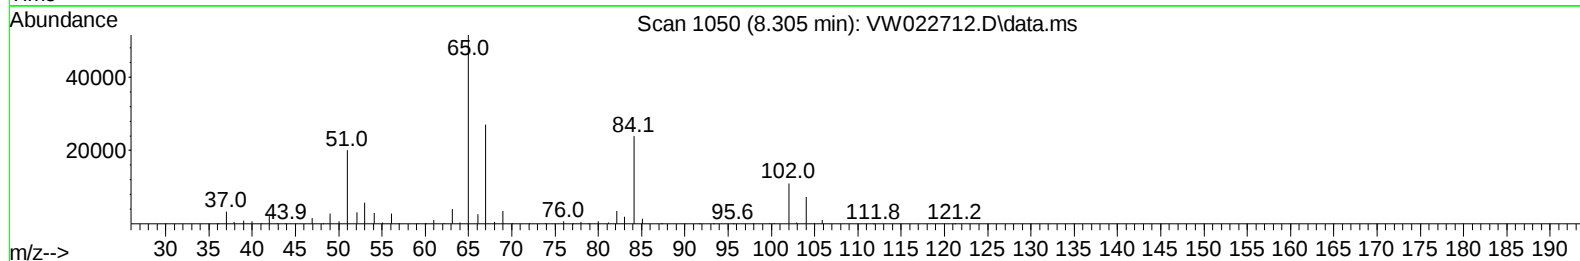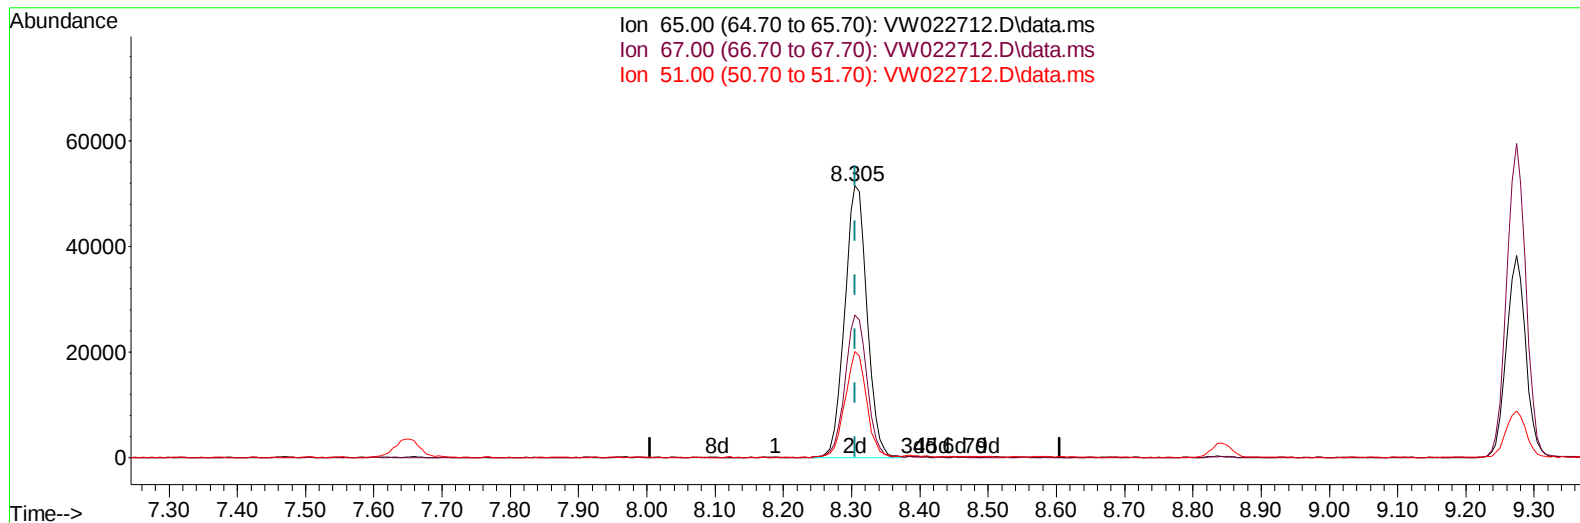

TIC: VW022712.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 24.45 ug/L m

response 116542

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.05#
51.00	99.30	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022712.D
 Acq On : 29 Apr 2022 21:41
 Operator : SY/VA
 Sample : N2638-01
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXKZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 30 02:00:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 30 01:41:13 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	266915	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	238461	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93625	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	114177	19.350	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.400%	
7) Chloroethane-d5	2.885	69	78698	21.281	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	85.120%	
11) 1,1-Dichloroethene-d2	4.019	63	124828	16.310	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	65.240%	
21) 2-Butanone-d5	7.079	46	48067	46.659	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	93.320%	
24) Chloroform-d	7.646	84	207789	24.906	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.640%	
26) 1,2-Dichloroethane-d4	8.305	65	116542m	24.449	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.800%	
32) Benzene-d6	8.274	84	388173	26.644	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	106.560%	
36) 1,2-Dichloropropane-d6	9.274	67	116596	27.655	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	110.600%	
41) Toluene-d8	10.323	98	343023	24.040	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	96.160%	
43) trans-1,3-Dichloroprop...	10.573	79	41662	20.938	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.760%	
47) 2-Hexanone-d5	10.920	63	38320	48.851	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	97.700%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	98237	27.403	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	109.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152	82825	24.976	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.920%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022712.D
Acq On : 29 Apr 2022 21:41
Operator : SY/VA
Sample : N2638-01
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXKZ2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/04/2022
Supervised By :Semsettin Yesilyurt 05/04/2022

Quant Time: Apr 30 02:00:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 30 01:41:13 2022
Response via : Initial Calibration

