

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
 Data File : VW022693.D
 Acq On : 29 Apr 2022 12:21
 Operator : SY/VA
 Sample : N2603-12RE
 Misc : 6.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW493RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: Apr 29 22:24:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 29 22:19:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	248703	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	151557	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	29555	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	74718	13.590	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.360%		
7) Chloroethane-d5	2.885	69	63648	18.471	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.880%		
11) 1,1-Dichloroethene-d2	4.019	63	78021m	10.941	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	43.760%#		
21) 2-Butanone-d5	7.074	46	73871	76.958	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	153.920%#		
24) Chloroform-d	7.647	84	173701	22.345	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.360%		
26) 1,2-Dichloroethane-d4	8.305	65	101346	22.818	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.280%		
32) Benzene-d6	8.275	84	277520	29.971	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	119.880%		
36) 1,2-Dichloropropane-d6	9.275	67	94858	35.400	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	141.600%#		
41) Toluene-d8	10.323	98	189291	20.873	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	83.480%		
43) trans-1,3-Dichloroprop...	10.579	79	25494	20.159	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.640%		
47) 2-Hexanone-d5	10.921	63	50075	100.442	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	200.880%#		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	97940	42.986	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	171.960%#		
66) 1,2-Dichlorobenzene-d4	13.853	152	31957	30.527	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	122.120%#		
Target Compounds					Qvalue	
13) Acetone	4.129	43	4159	6.364	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW042922\
Data File : VW022693.D
Acq On : 29 Apr 2022 12:21
Operator : SY/VA
Sample : N2603-12RE
Misc : 6.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW493RE

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/01/2022
Supervised By : Mahesh Dadoda 05/04/2022


Quant Time: Apr 29 22:24:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 29 22:19:25 2022
Response via : Initial Calibration

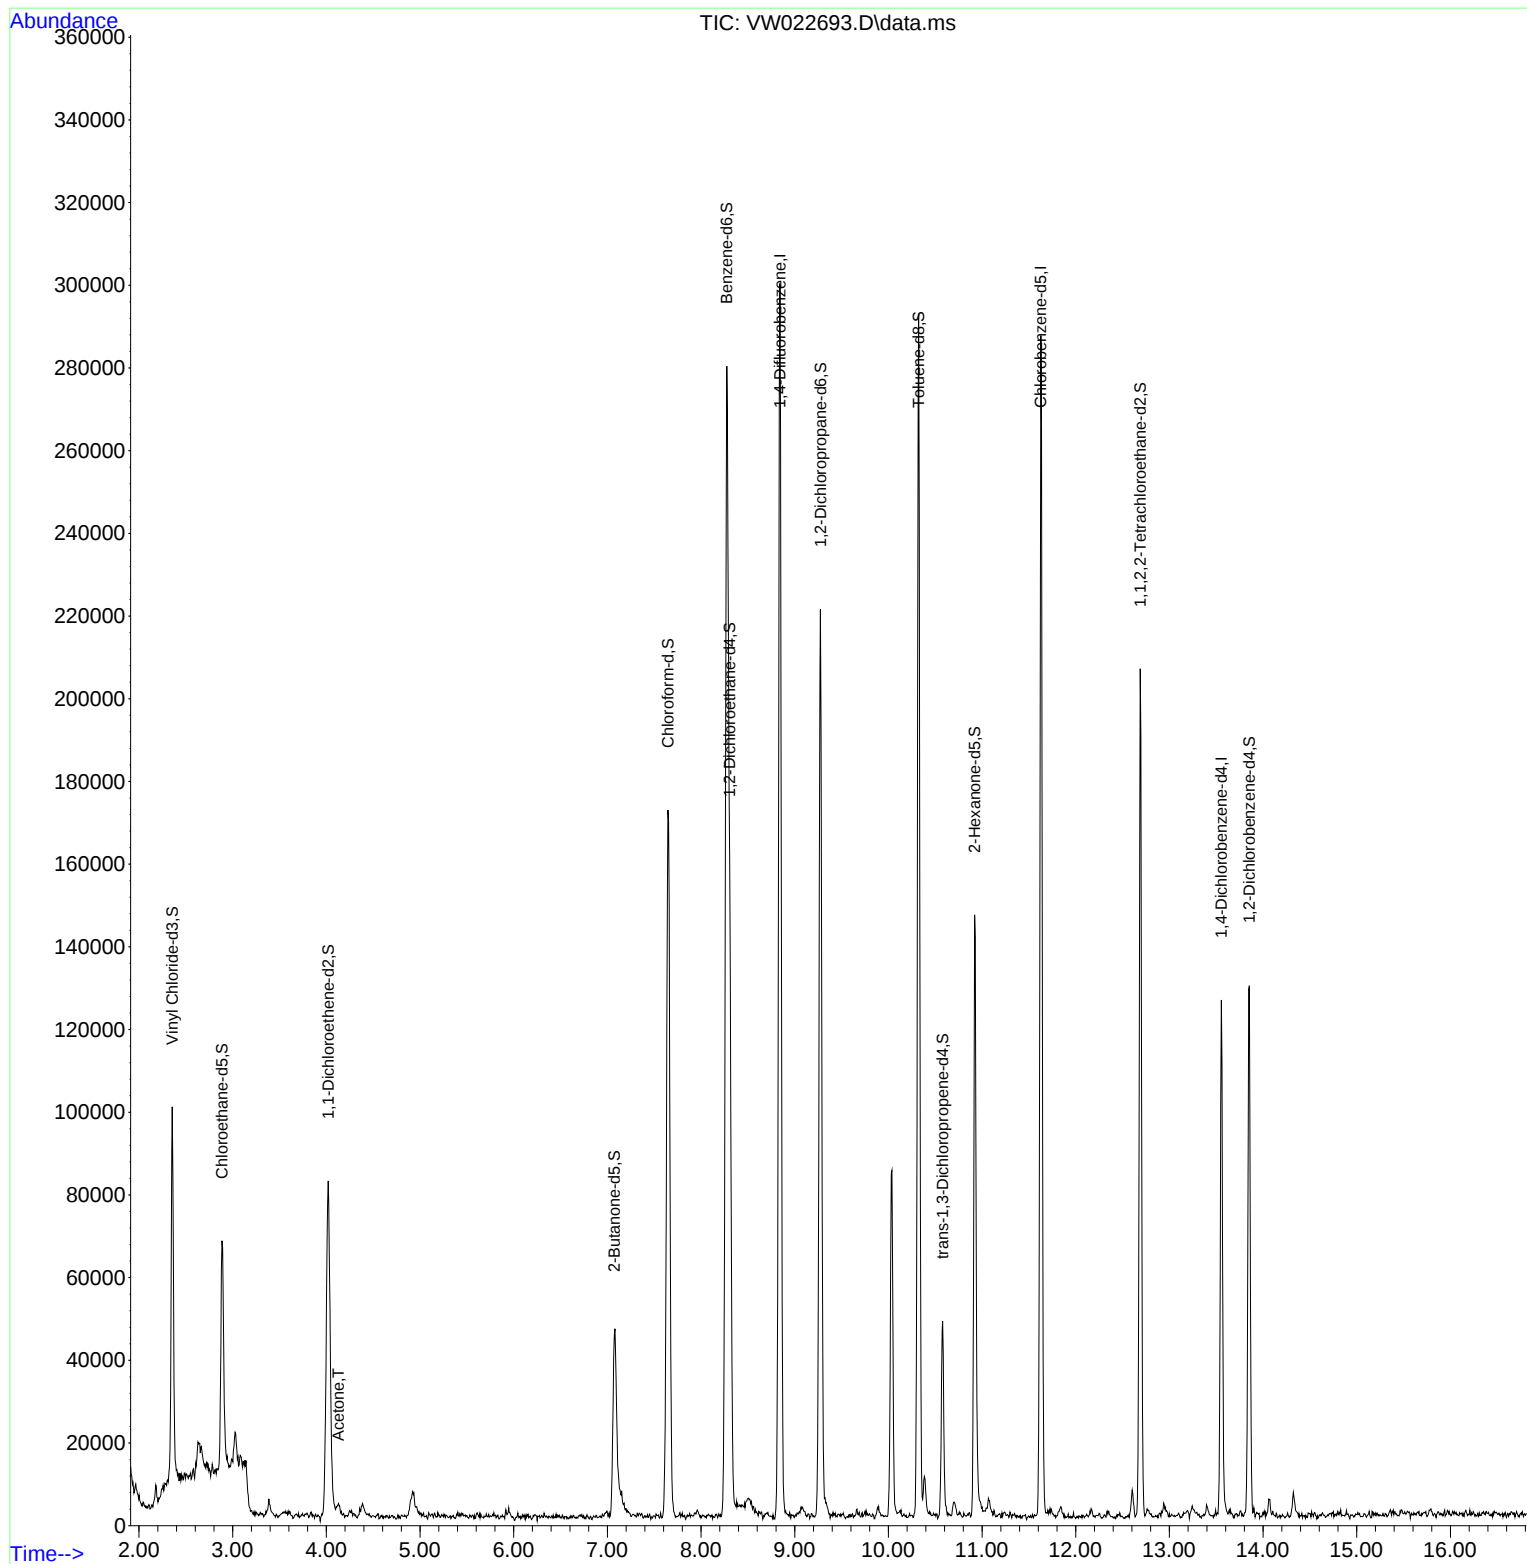

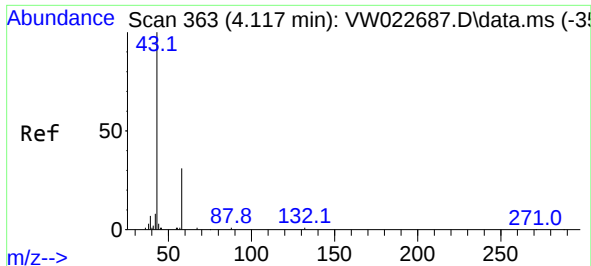

#13
 Acetone
 Concen: 6.364 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW022693.D
 Acq: 29 Apr 2022 12:21

Instrument :
 MSVOA_W
 ClientSampleId :
 EW493RE

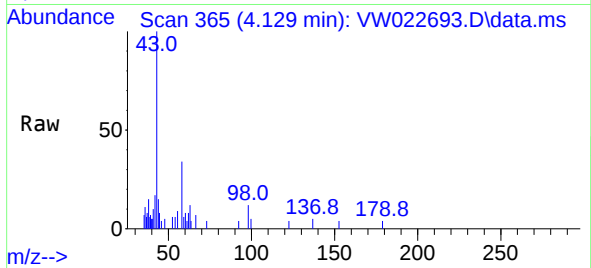

Tgt Ion: 43 Resp: 4159
 Ion Ratio Lower Upper
 43 100
 58 25.1 0.0 57.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/01/2022
 Supervised By :Mahesh Dadoda 05/04/2022

