

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW050119\
 Data File : VW010229.D
 Acq On : 01 May 2019 00:29
 Operator : SY/VA
 Sample : VW0501SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK19

Quant Time: May 01 07:37:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 01 03:52:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	625838	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	599248	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	265900	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	126830	17.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.44%
7) Chloroethane-d5	2.89	69	110238	18.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.76%
10) 1,1-Dichloroethene-d2	4.01	63	229457	14.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.12%
20) 2-Butanone-d5	7.07	46	135147	51.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.22%
24) Chloroform-d	7.64	84	349698	21.56	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.24%
26) 1,2-Dichloroethane-d4	8.31	65	224408	24.08	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.32%
29) Benzene-d6	8.27	84	659027	20.42	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.68%
33) 1,2-Dichloropropane-d6	9.27	67	217476	21.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.28%
37) Toluene-d8	10.32	98	566801	19.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.28%
38) trans-1,3-Dichloropropene-	10.57	79	91339	19.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.64%
39) 2-Hexanone-d5	10.93	63	99248	46.85	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.70%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	191664	22.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	211905	21.45	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.80%


Target Compounds					Qvalue
13) Acetone	4.12	43	6175	2.984 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW050119\
Data File : VW010229.D
Acq On : 01 May 2019 00:29
Operator : SY/VA
Sample : VW0501SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK19

Quant Time: May 01 07:37:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 03:52:51 2019
Response via : Initial Calibration

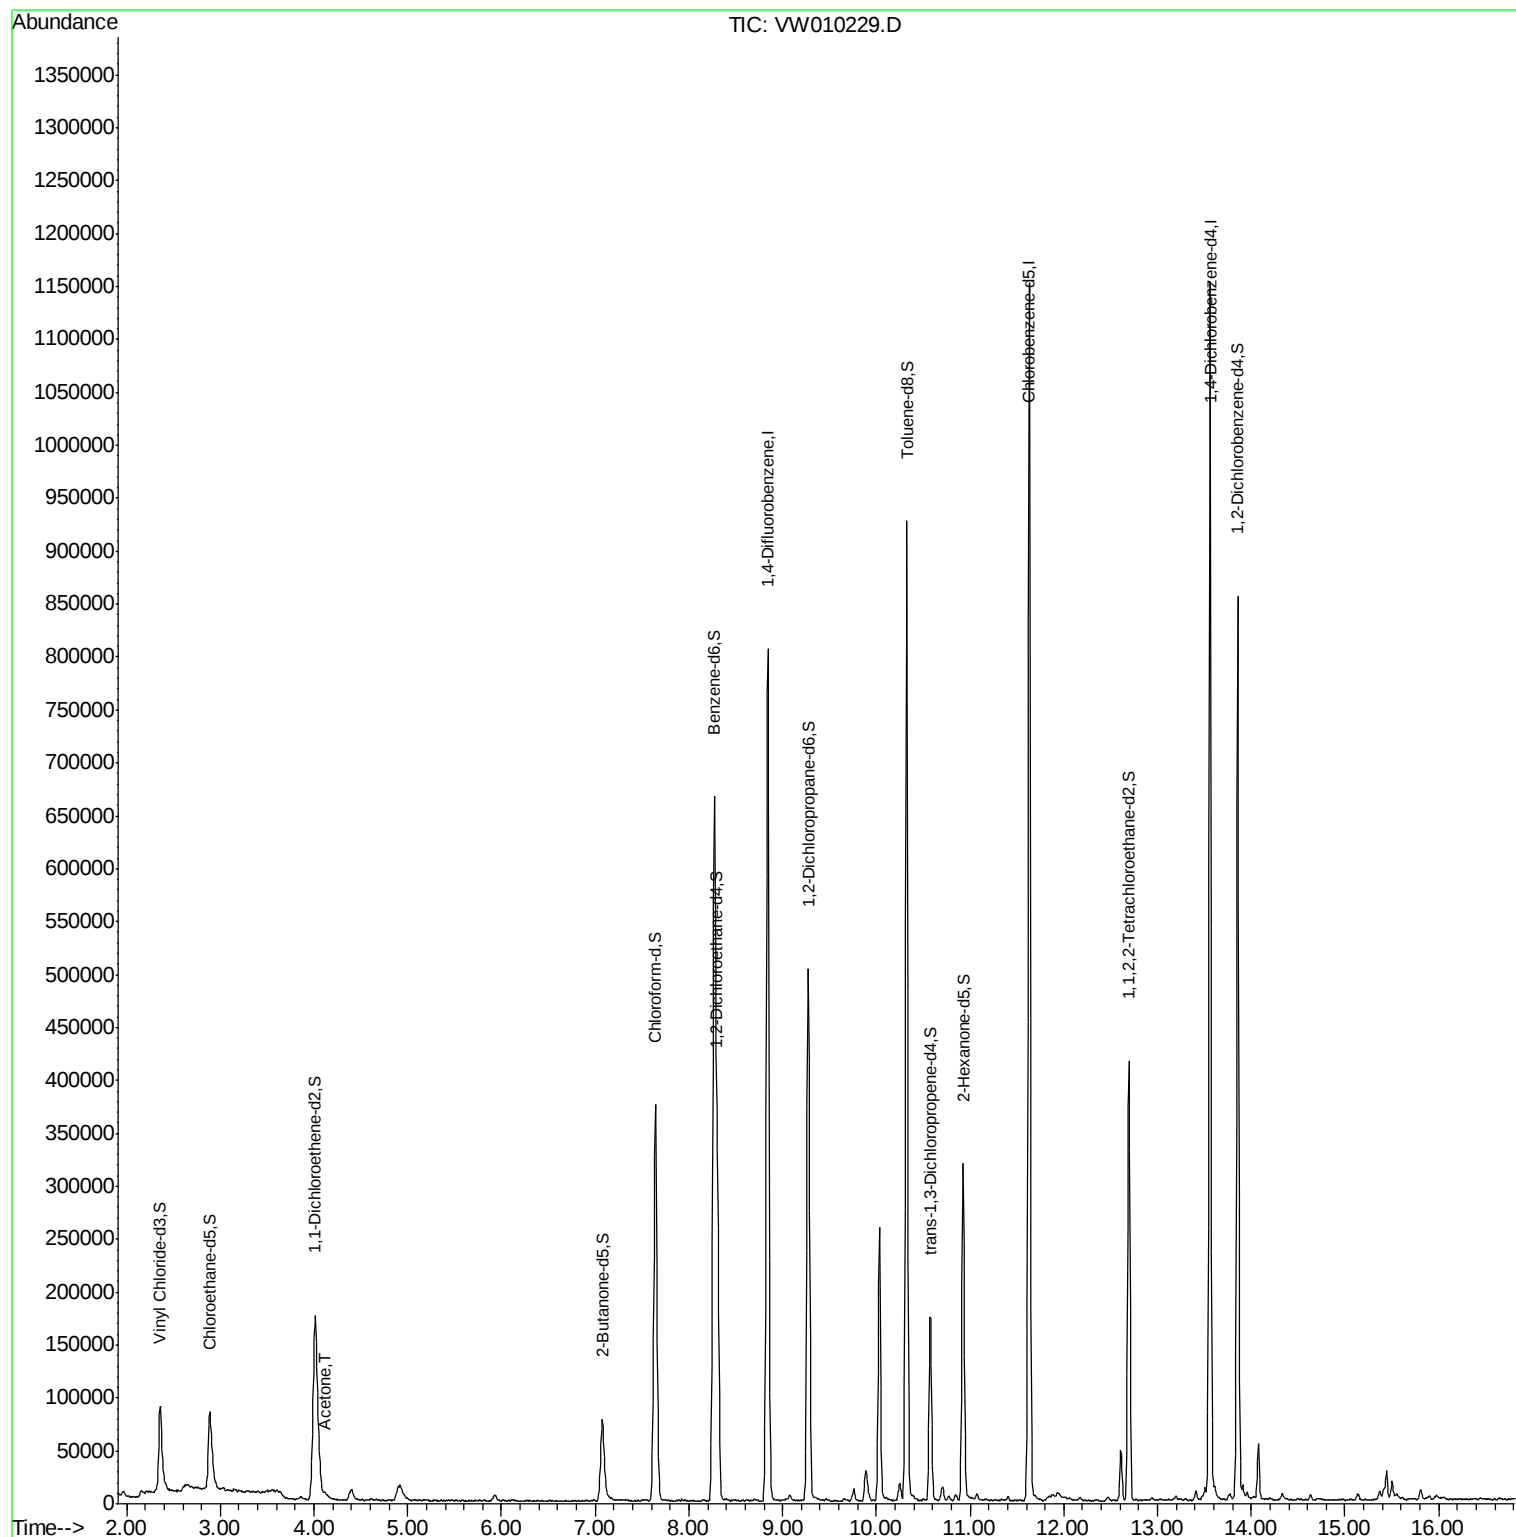

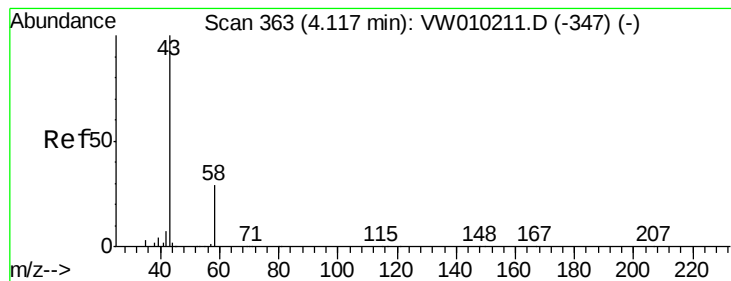

#13
 Acetone
 Concen: 2.984 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. 0.01 min
 Lab File: VW010229.D
 Acq: 01 May 2019 00:29

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK19

Tgt Ion: 43 Resp: 6175
 Ion Ratio Lower Upper
 43 100
 58 20.6 0.0 59.8

