

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW050119\
 Data File : VW010233.D
 Acq On : 01 May 2019 02:51
 Operator : SY/VA
 Sample : K2602-11
 Misc : 3.61G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFH70

Quant Time: May 01 07:38:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 01 03:52:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	497877	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	486296	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	205026	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	87391	15.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.88%
7) Chloroethane-d5	2.89	69	86379	18.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.60%
10) 1,1-Dichloroethene-d2	4.01	63	175037	13.94	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.76%
20) 2-Butanone-d5	7.07	46	91735	44.04	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.08%
24) Chloroform-d	7.65	84	321888	24.95	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.80%
26) 1,2-Dichloroethane-d4	8.45	65	71	0.01	ug/L	0.14
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.04%#
29) Benzene-d6	8.27	84	557520	21.29	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.16%
33) 1,2-Dichloropropane-d6	9.27	67	195894	23.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.80%
37) Toluene-d8	10.32	98	475641	19.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.88%
38) trans-1,3-Dichloropropene-	10.58	79	69353	18.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.60%
39) 2-Hexanone-d5	10.93	63	65096	37.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	152348	21.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.24%
61) 1,2-Dichlorobenzene-d4	13.86	152	189772	24.92	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.68%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.12	43	4870	2.958	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW050119\
Data File : VW010233.D
Acq On : 01 May 2019 02:51
Operator : SY/VA
Sample : K2602-11
Misc : 3.61G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFH70

Quant Time: May 01 07:38:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 03:52:51 2019
Response via : Initial Calibration

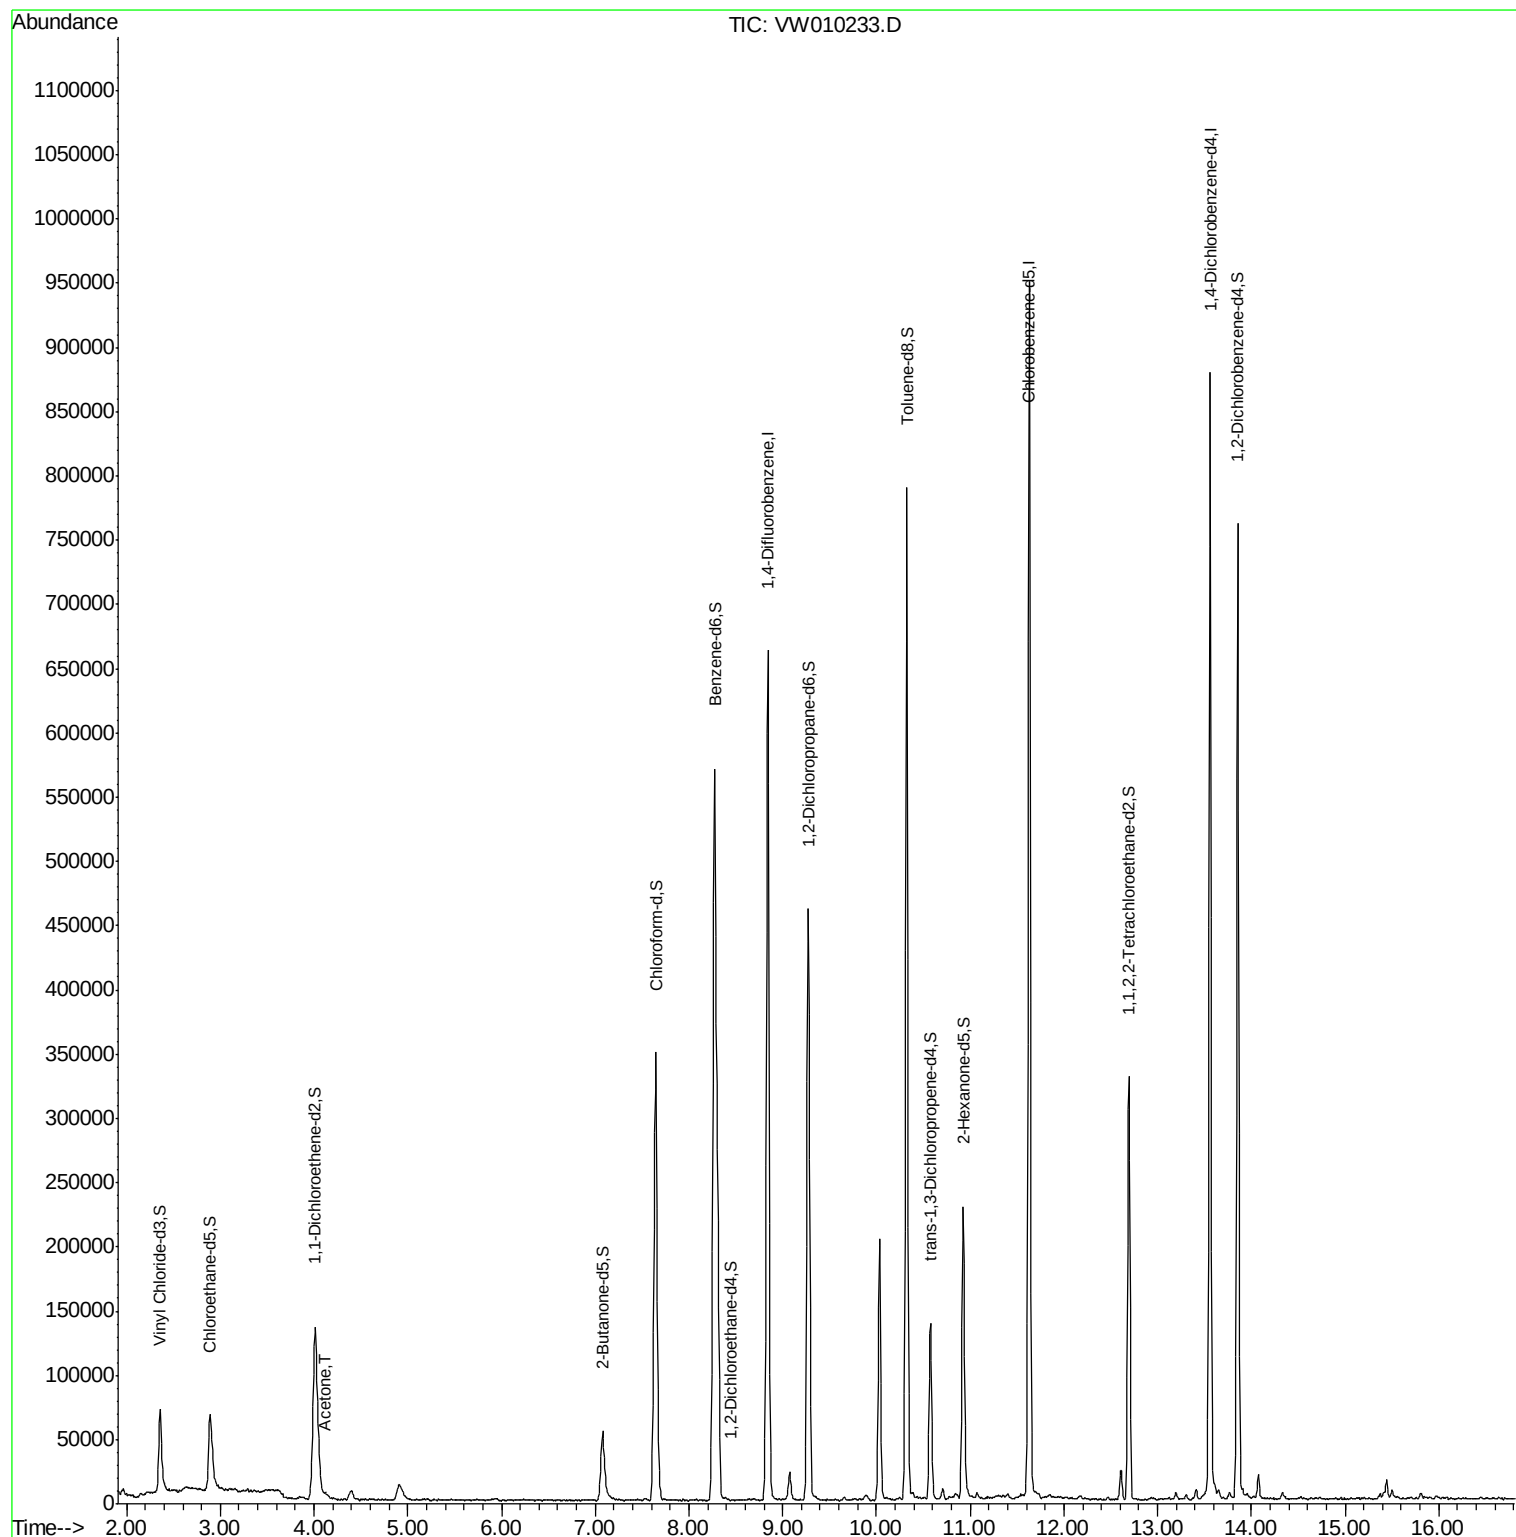

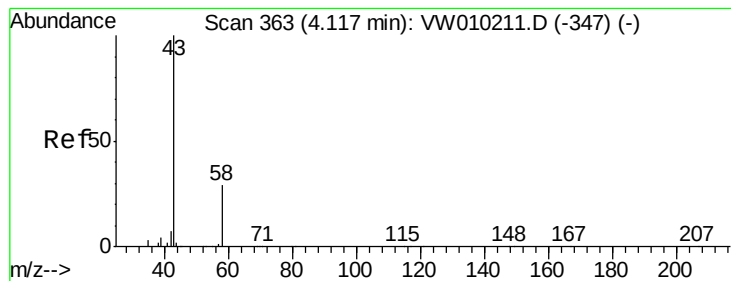

#13

Acetone

Concen: 2.958 ug/L

RT: 4.12 min Scan# 363

Delta R.T. -0.00 min

Lab File: VW010233.D

Acq: 01 May 2019 02:51

Instrument :
MSVOA_W
ClientSampleId :
BFH70

Tgt Ion: 43 Resp: 4870

Ion Ratio Lower Upper

43 100

58 24.8 0.0 59.8

