

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW050119\
 Data File : VW010244.D
 Acq On : 01 May 2019 13:17
 Operator : SY/VA
 Sample : VW0501SBL02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK20

Quant Time: May 02 03:45:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 02 03:31:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	615959	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	578487	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	256187	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	155570	22.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.04%
7) Chloroethane-d5	2.89	69	128466	22.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.68%
10) 1,1-Dichloroethene-d2	4.01	63	275236	17.71	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.84%
20) 2-Butanone-d5	7.07	46	146862	56.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.96%
24) Chloroform-d	7.64	84	388270	24.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.28%
26) 1,2-Dichloroethane-d4	8.30	65	240253	26.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.80%
29) Benzene-d6	8.27	84	742148	23.83	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.32%
33) 1,2-Dichloropropane-d6	9.27	67	240370	24.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.80%
37) Toluene-d8	10.32	98	651228	22.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.96%
38) trans-1,3-Dichloropropene-	10.58	79	103108	23.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.00%
39) 2-Hexanone-d5	10.93	63	105492	51.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	208327	25.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.28%
61) 1,2-Dichlorobenzene-d4	13.86	152	234752	24.67	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.68%


Target Compounds					Ovalue
13) Acetone	4.11	43	4863	2.388 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW050119\
Data File : VW010244.D
Acq On : 01 May 2019 13:17
Operator : SY/VA
Sample : VW0501SBL02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK20

Quant Time: May 02 03:45:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 03:31:19 2019
Response via : Initial Calibration

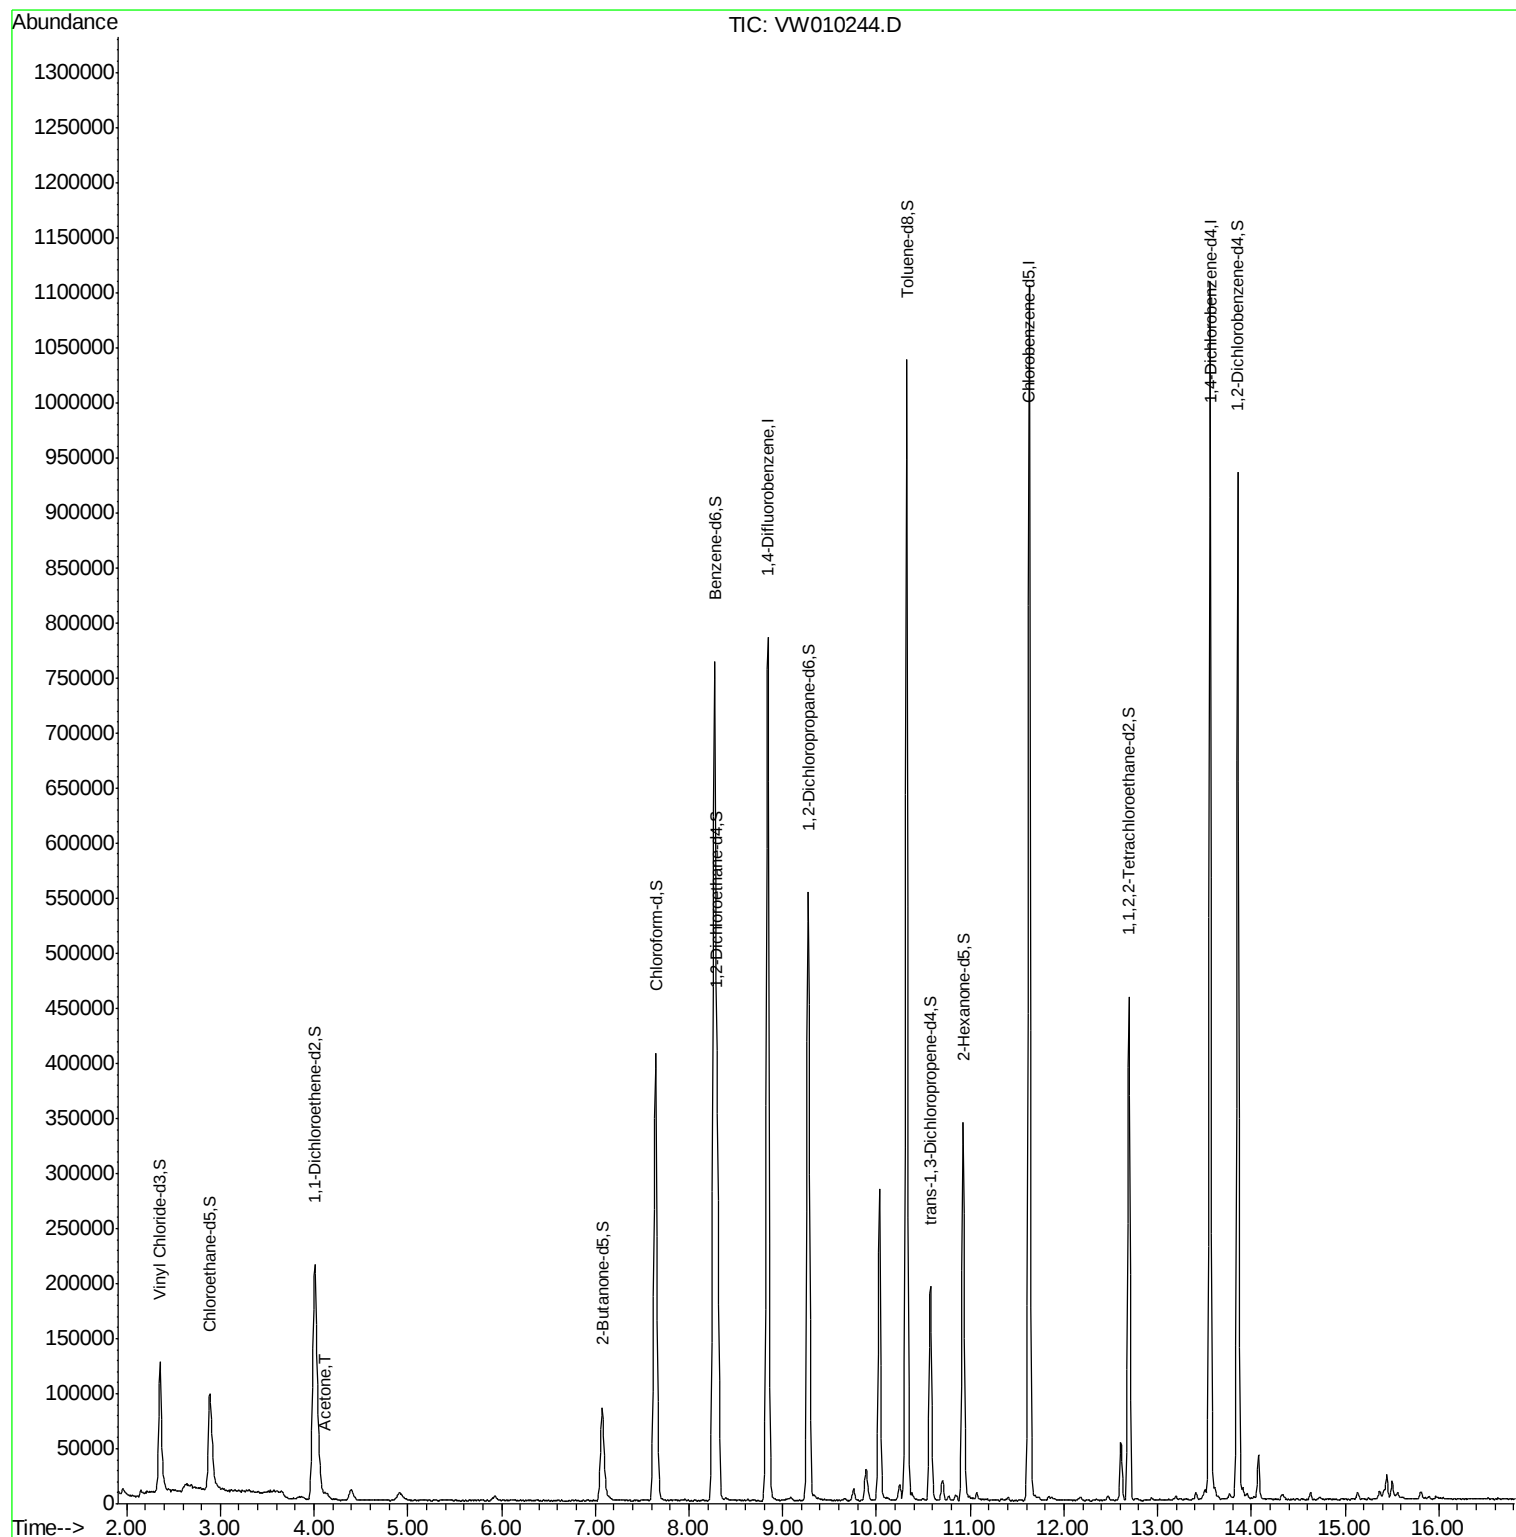

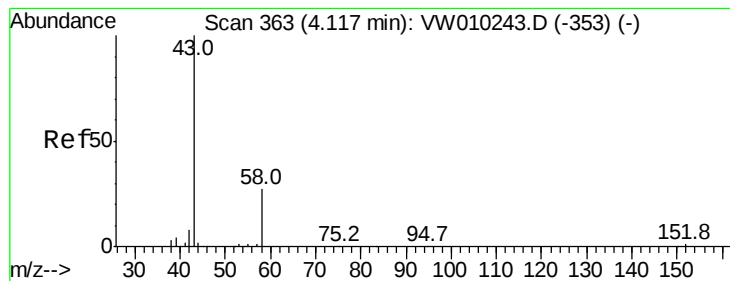

#13

Acetone

Concen: 2.388 ug/L

RT: 4.11 min Scan# 362

Delta R.T. -0.01 min

Lab File: VW010244.D

Acq: 01 May 2019 13:17

Instrument :

MSVOA_W

ClientSampleId :

VBLK20

Tot Ion: 43 Resp: 4863

Ion Ratio Lower Upper

43 100

58 23.4 0.0 59.8

