

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW050119\
 Data File : VW010248.D
 Acq On : 01 May 2019 15:23
 Operator : SY/VA
 Sample : K2602-09
 Misc : 3.30G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFH58

Quant Time: May 02 03:45:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 02 03:31:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	479593	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	417676	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	156302	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	88148	16.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.80%
7) Chloroethane-d5	2.89	69	79582	17.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.36%
10) 1,1-Dichloroethene-d2	4.01	63	168839	13.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.84%
20) 2-Butanone-d5	7.08	46	75075	37.41	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.82%
24) Chloroform-d	7.65	84	235290	18.93	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.72%
26) 1,2-Dichloroethane-d4	8.31	65	137296	19.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.92%
29) Benzene-d6	8.27	84	403235	17.93	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.72%
33) 1,2-Dichloropropane-d6	9.27	67	133235	18.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.84%
37) Toluene-d8	10.32	98	345209	16.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.52%
38) trans-1,3-Dichloropropene-	10.58	79	48657	15.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	60.12%
39) 2-Hexanone-d5	10.93	63	46598	31.56	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	108301	18.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	72.20%
61) 1,2-Dichlorobenzene-d4	13.86	152	108656	18.71	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.84%#


Target Compounds				Ovalue
13) Acetone	4.12	43	4619	2.913 ug/L 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW050119\
Data File : VW010248.D
Acq On : 01 May 2019 15:23
Operator : SY/VA
Sample : K2602-09
Misc : 3.30G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFH58

Quant Time: May 02 03:45:50 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 03:31:19 2019
Response via : Initial Calibration

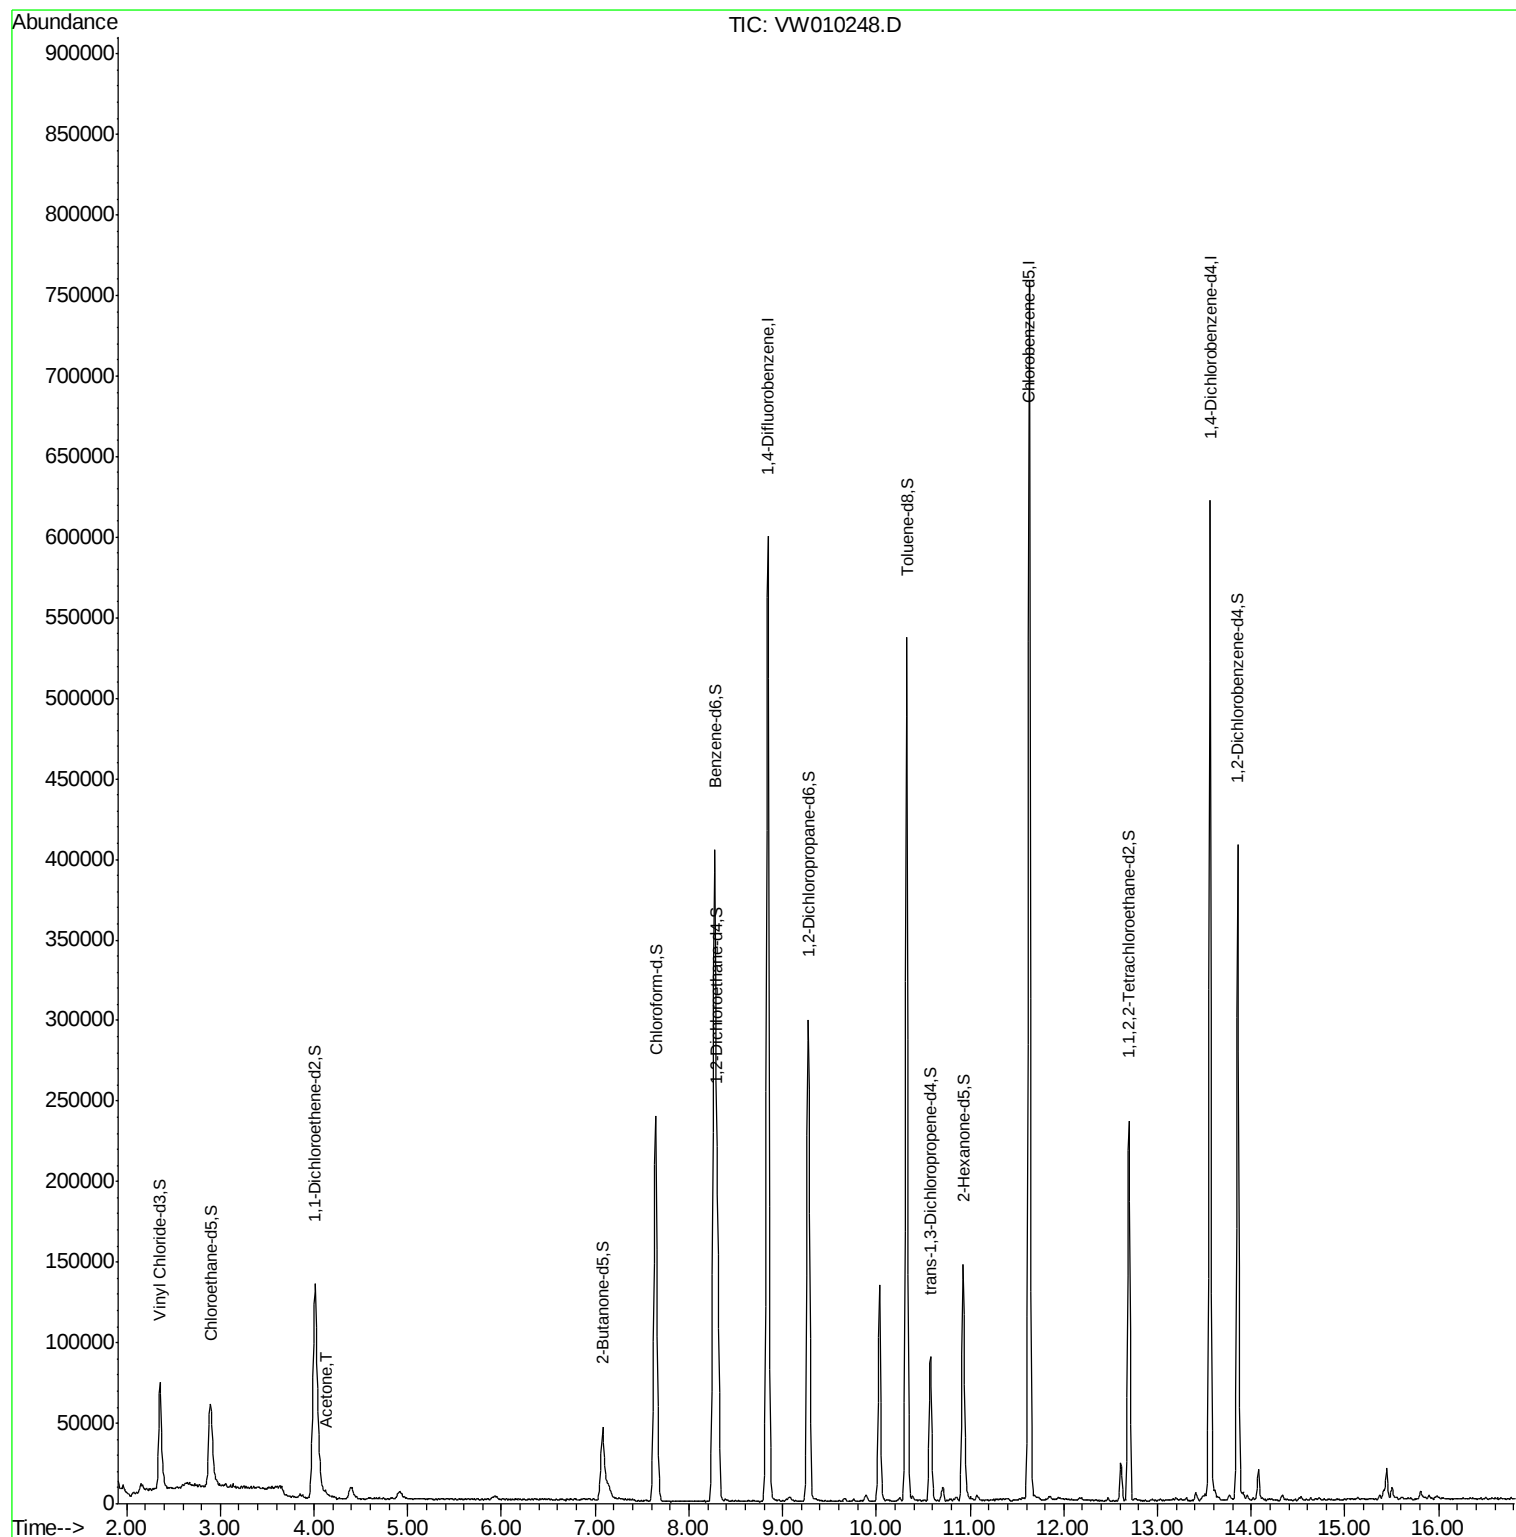

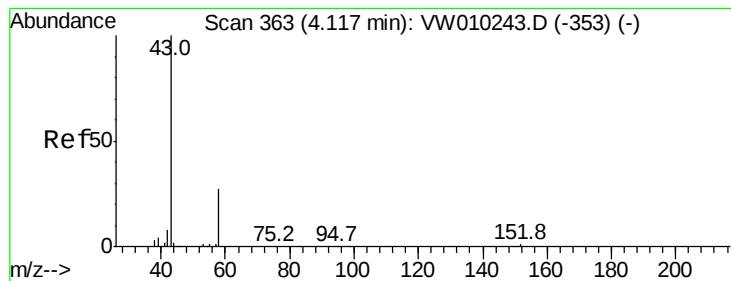

#13
 Acetone
 Concen: 2.913 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. 0.01 min
 Lab File: VW010248.D
 Acq: 01 May 2019 15:23

Instrument :
 MSVOA_W
 ClientSampleId :
 BFH58

Tot Ion: 43 Resp: 4619
 Ion Ratio Lower Upper
 43 100
 58 15.4 0.0 59.8

