

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050119\

Quantitation Report (LSC Reviewed)

Data File : VW010240.D

Acq On : 01 May 2019 07:06

Operator : SY/VA

Sample : K2604-11

Misc : 5.10G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

Client Sample ID :

GAJ85

Quant Time: May 02 22:39:58 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M

Quant Title : VOC Analysis


QLast Update : Wed May 01 07:37:51 2019

Response via : Initial Calibration

Manual Integrations
APPROVED

sam

5/7/2019 9:20:11 AM

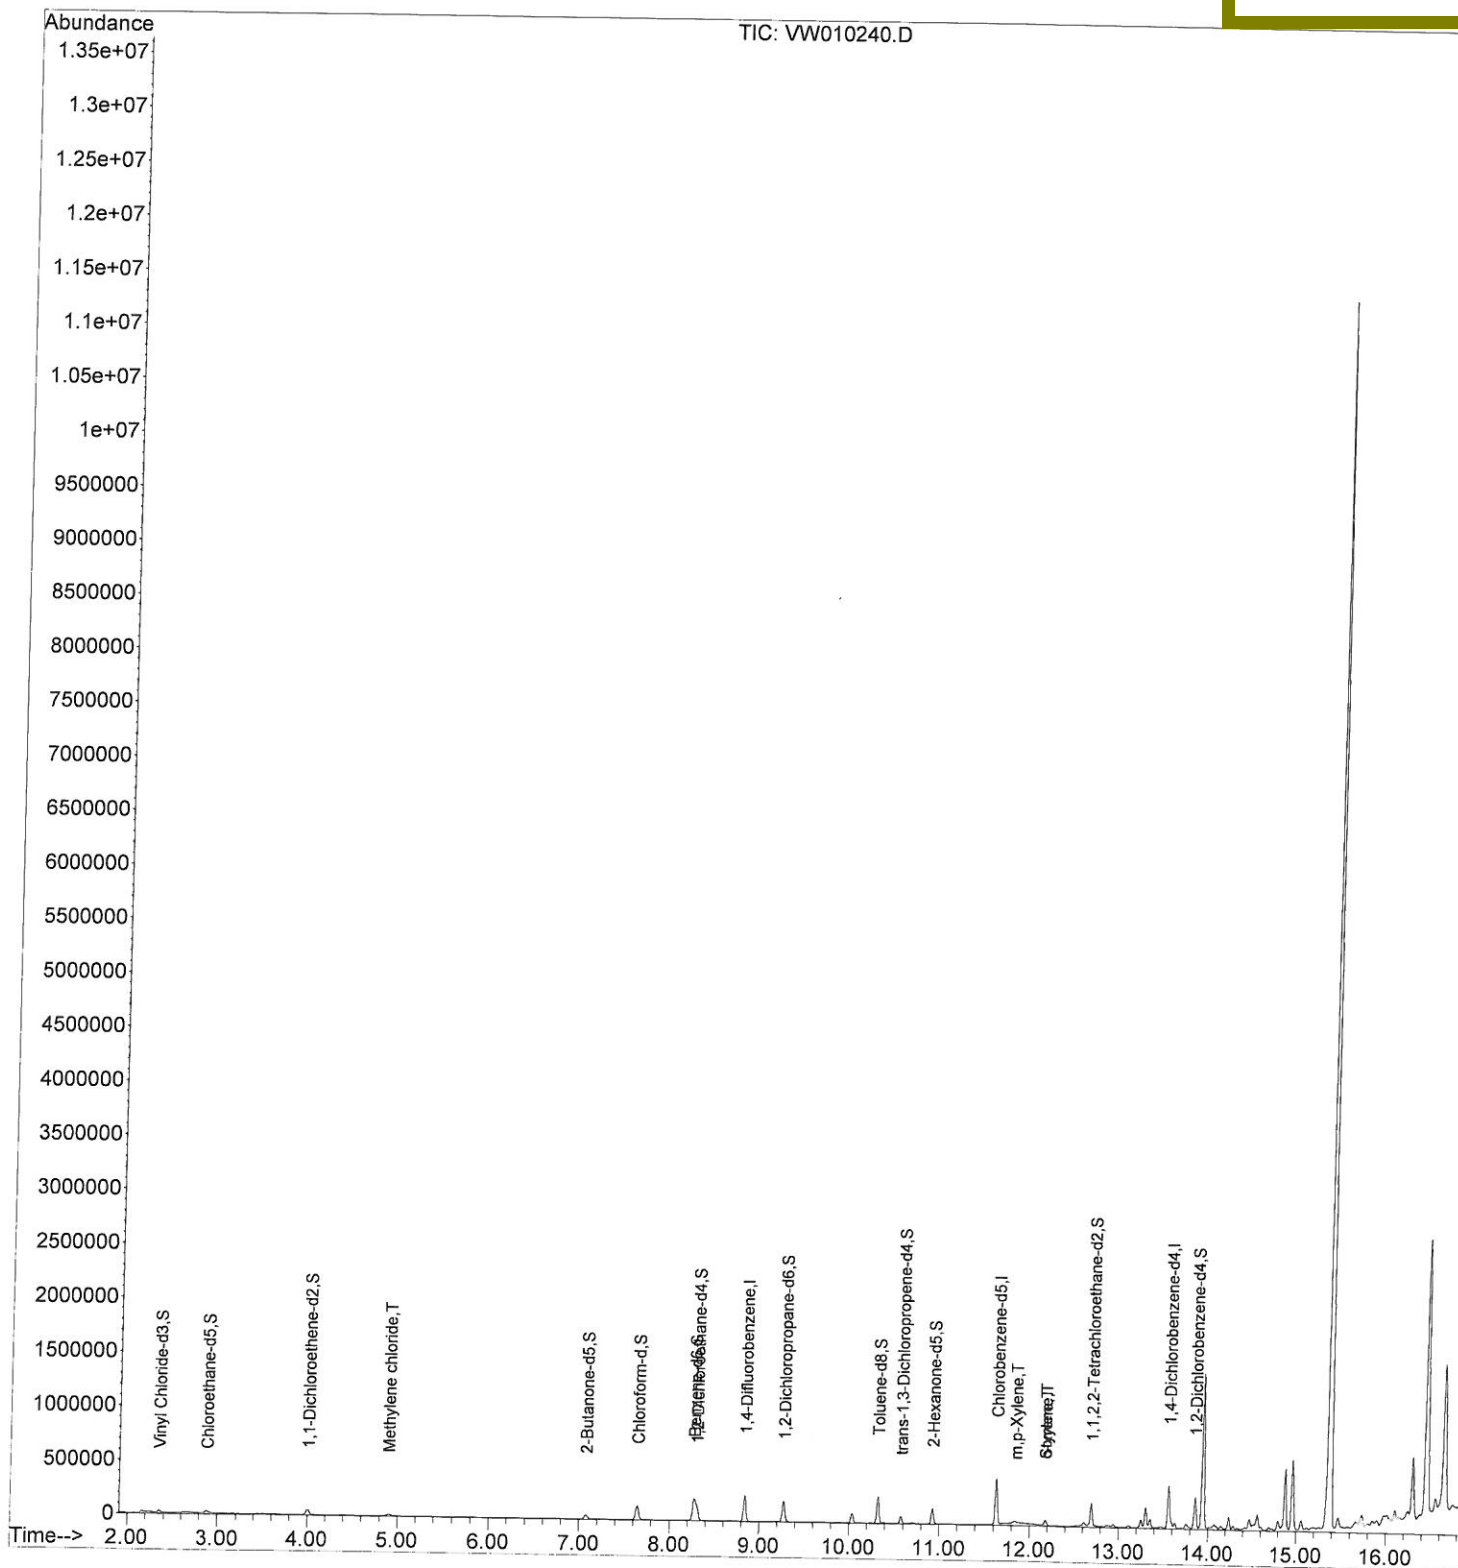

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050119\
Quantitation Report (Qedit)




Data File : VW010240.D
Acq On : 01 May 2019 07:06
Operator : SY/VA
Sample : K2604-11
Misc : 5.10G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
GAJ85

Quant Time: May 01 08:49:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 07:37:51 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

sam
5/7/2019 9:20:11 AM

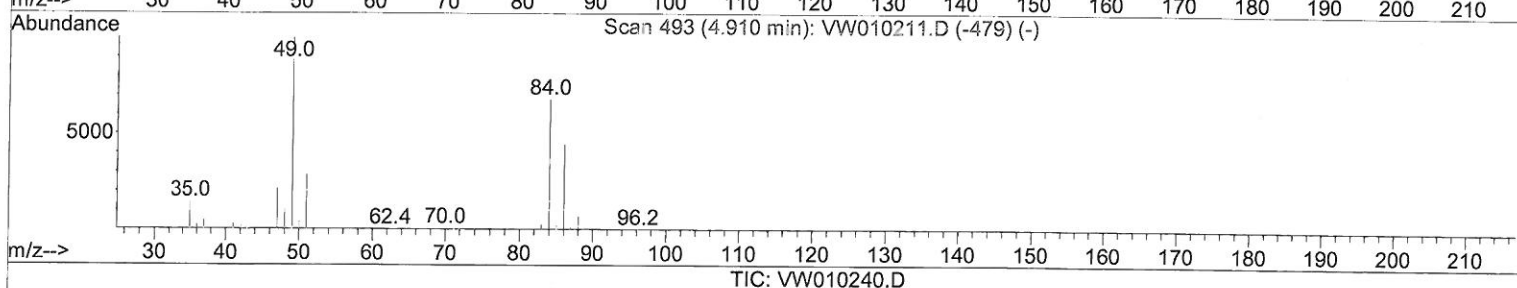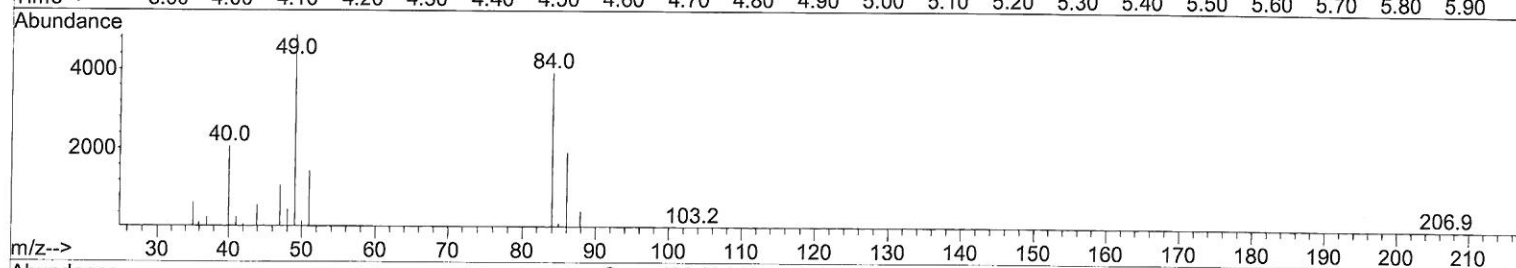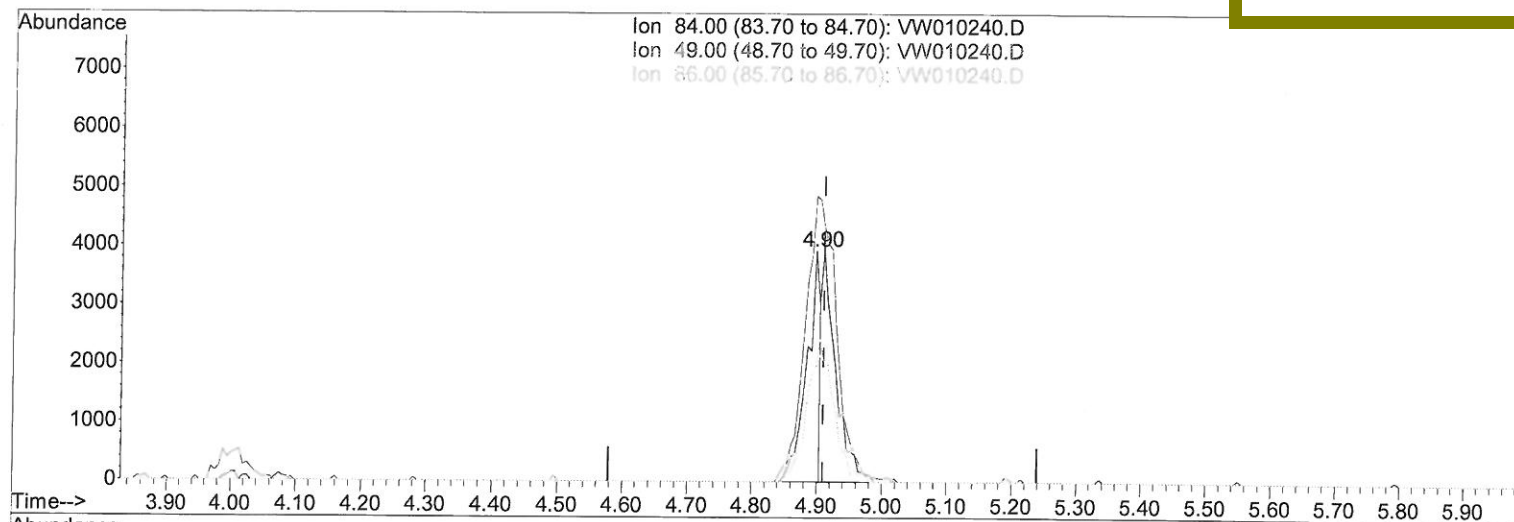

(16) Methylene chloride (T)

4.897min (-0.012) 1.79ug/L

response 5539

Ion	Exp%	Act%
84.00	100	100
49.00	128.90	123.80
86.00	66.20	48.99
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050119\
Quantitation Report (Qedit)




Data File : VW010240.D
Acq On : 01 May 2019 07:06
Operator : SY/VA
Sample : K2604-11
Misc : 5.10G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
GAJ85

Quant Time: May 01 08:49:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 07:37:51 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

sam
5/7/2019 9:20:11 AM

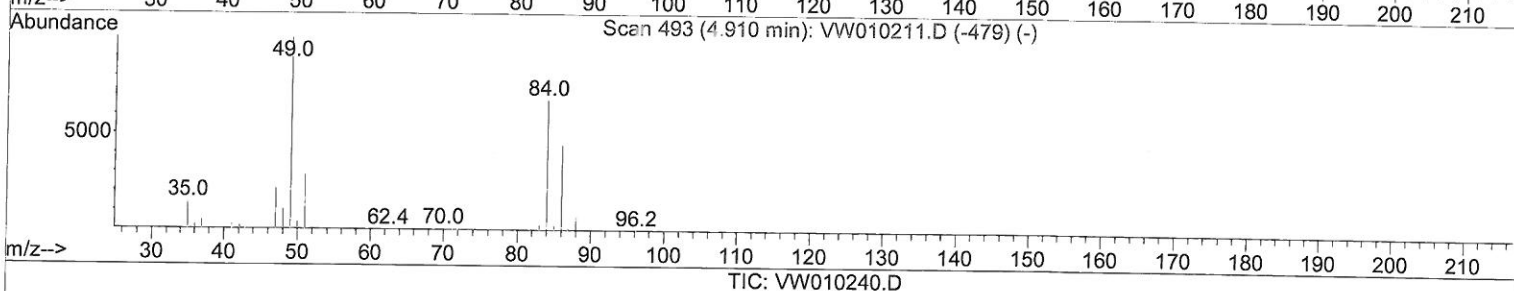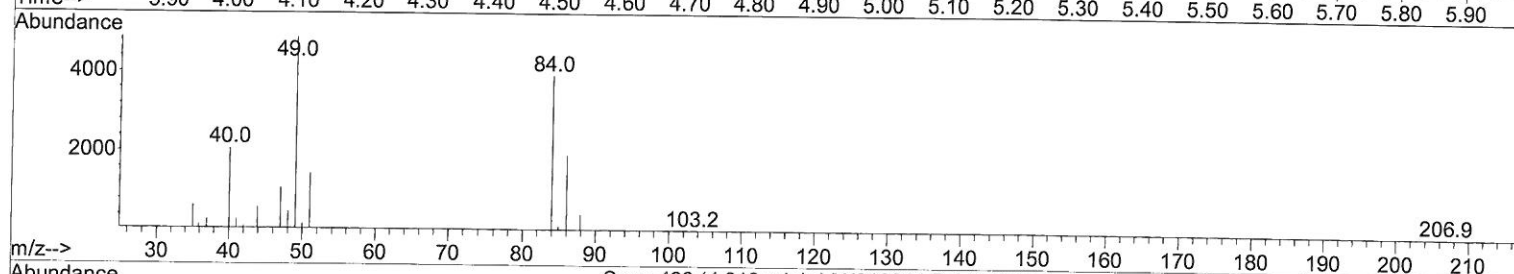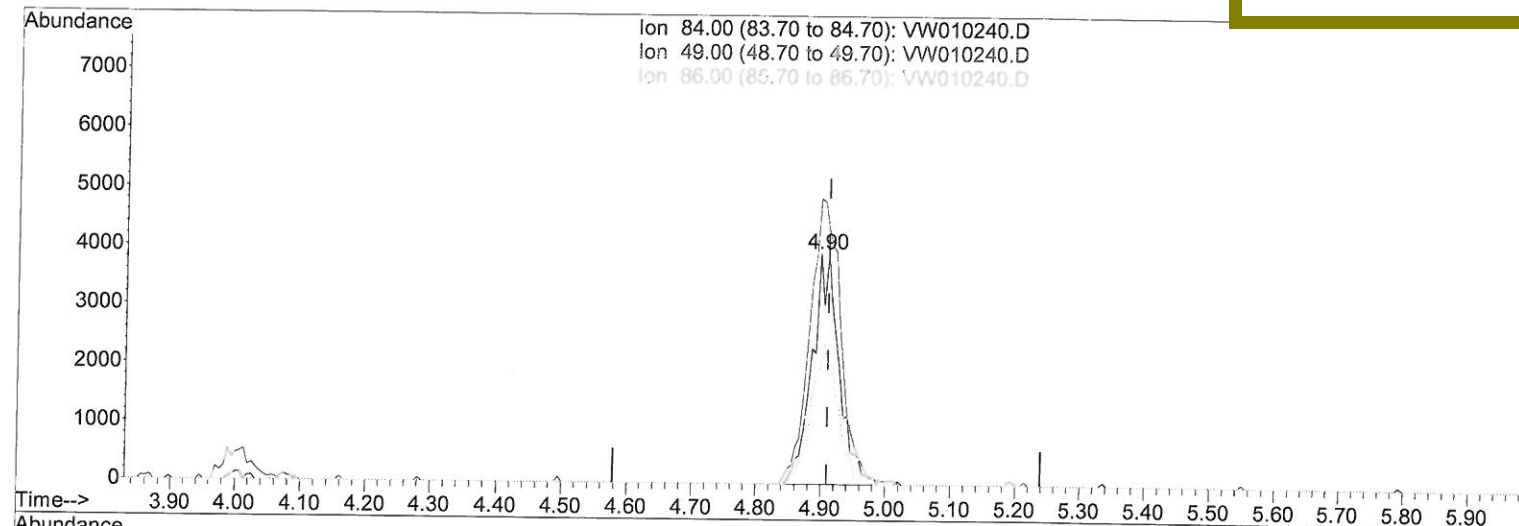

(16) Methylene chloride (T)

4.897min (-0.012) 3.68ug/L m

response 11352

Ion	Exp%	Act%
84.00	100	100
49.00	128.90	123.80
86.00	66.20	48.99
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050119\
Quantitation Report (LSC Reviewed)

Data File : VW010240.D
Acq On : 01 May 2019 07:06
Operator : SY/VA
Sample : K2604-11
Misc : 5.10G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
GAJ85

Quant Time: May 02 22:39:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM042919S.M
Quant Title : VOC Analysis
QLast Update : Wed May 01 07:37:51 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

sam
5/7/2019 9:20:11 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	185533	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	212479	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	99313	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	22694	10.78	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	43.12%
7) Chloroethane-d5	2.89	69	24690	14.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.24%
10) 1,1-Dichloroethene-d2	4.01	63	48405	10.34	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.36%#
20) 2-Butanone-d5	7.08	46	61681	79.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	158.92%#
24) Chloroform-d	7.64	84	123424	25.67	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.68%
26) 1,2-Dichloroethane-d4	8.31	65	92862	33.62	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	134.48%#
29) Benzene-d6	8.27	84	195659	17.10	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	68.40%
33) 1,2-Dichloropropane-d6	9.27	67	81936	22.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.68%
37) Toluene-d8	10.32	98	151343	14.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	58.20%
38) trans-1,3-Dichloropropene-	10.58	79	31605	19.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.76%
39) 2-Hexanone-d5	10.93	63	42631	56.76	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.52%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	100468	32.91	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	131.64%#
61) 1,2-Dichlorobenzene-d4	13.86	152	77283	20.95	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.80%

Target Compounds

16) Methylene chloride	4.90	84	11352m	3.677	ug/L	Qvalue
54) m,p-Xylene	11.84	106	4311	0.793	ug/L	97
55) o-xylene	12.17	106	3832	0.746	ug/L	96
56) Styrene	12.18	104	18686	2.099	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed