




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025789.D
Acq On : 02 May 2023 10:00
Operator : SY/MD
Sample : VW0502SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:21:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

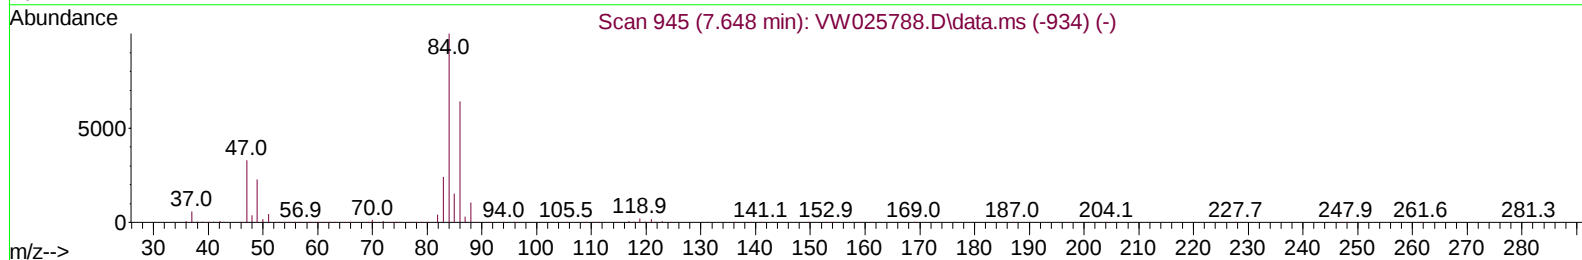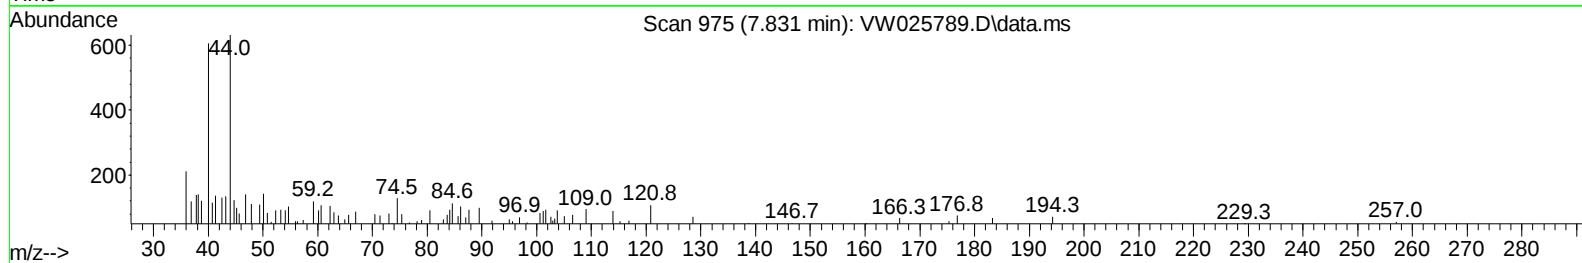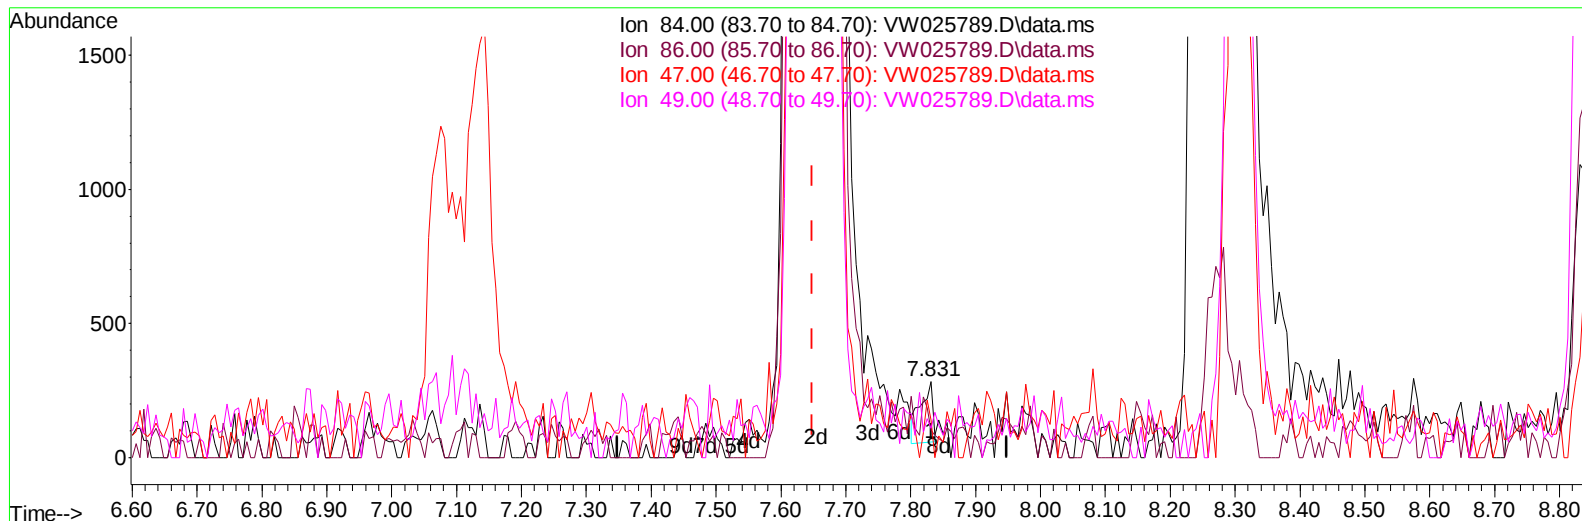

TIC: VW025789.D\data.ms

(24) Chloroform-d (S)

7.831min (+ 0.183) 0.02 ug/L

response 305

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.70	59.34
47.00	50.20	53.77
49.00	28.70	28.52




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025789.D
 Acq On : 02 May 2023 10:00
 Operator : SY/MD
 Sample : VW0502SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:21:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

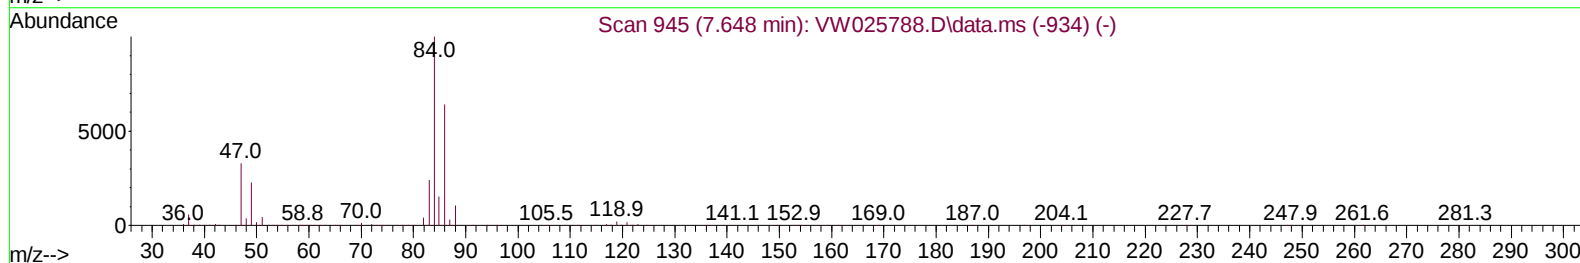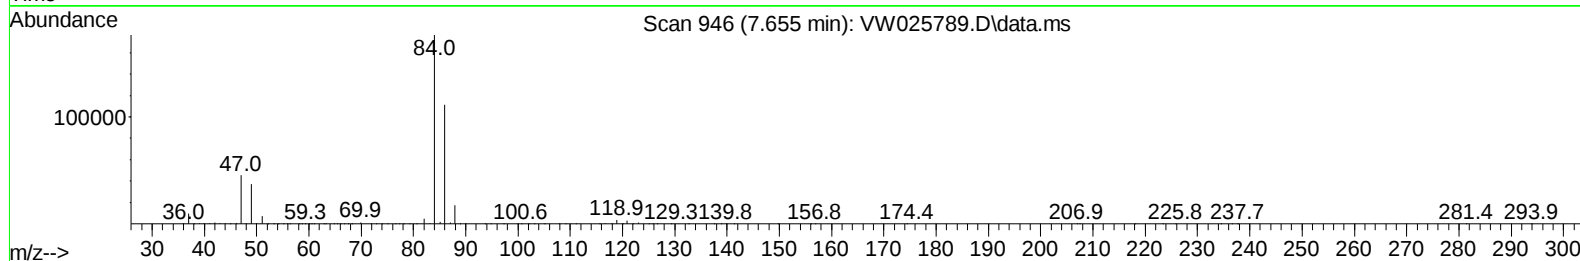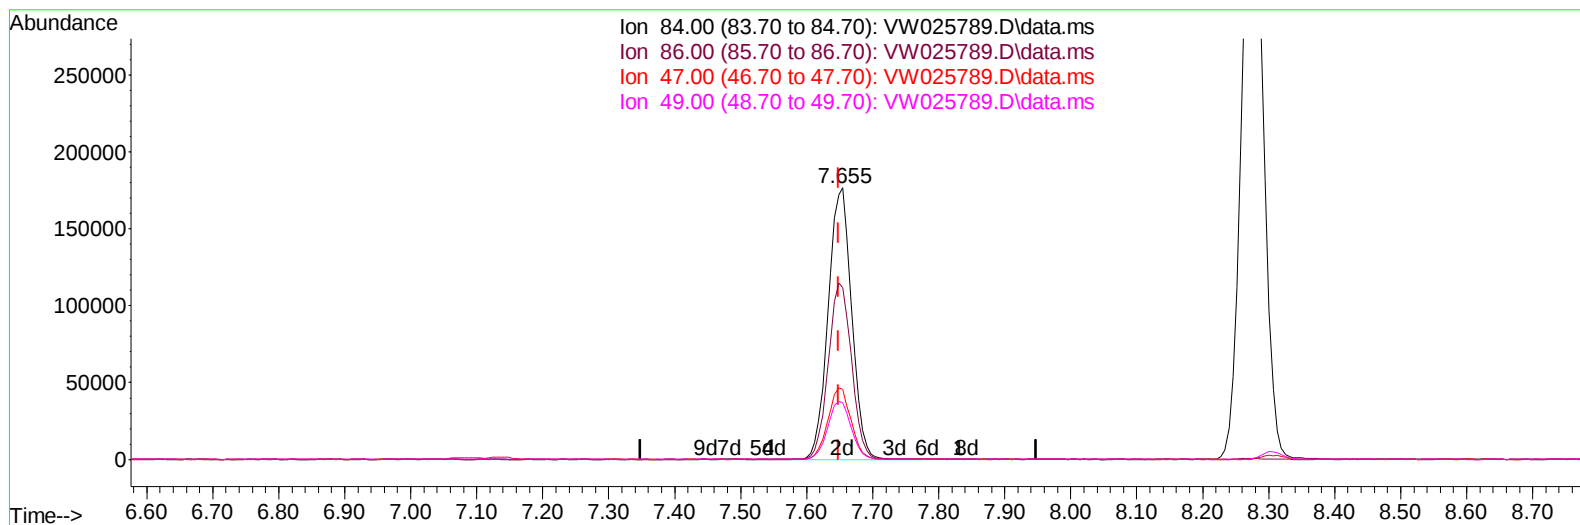

TIC: VW025789.D\data.ms

(24) Chloroform-d (S)

7.655min (+ 0.006) 25.41 ug/L m

response 436671

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.70	0.04#
47.00	50.20	0.04#
49.00	28.70	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025789.D
 Acq On : 02 May 2023 10:00
 Operator : SY/MD
 Sample : VW0502SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:21:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	595992	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	533535	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	239447	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	247305	29.282	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	117.120%	
7) Chloroethane-d5	2.899	69	180230	28.785	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	115.120%	
11) 1,1-Dichloroethene-d2	4.021	65	114761	27.137	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	108.560%	
21) 2-Butanone-d5	7.081	46	127077	45.514	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.020%	
24) Chloroform-d	7.655	84	436671m	25.409	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	101.640%	
26) 1,2-Dichloroethane-d4	8.307	65	248267	25.547	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	102.200%	
32) Benzene-d6	8.276	84	924654	26.523	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	106.080%	
36) 1,2-Dichloropropane-d6	9.276	67	289402	25.945	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	103.800%	
41) Toluene-d8	10.325	98	820886	26.406	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	105.640%	
43) trans-1,3-Dichloroprop...	10.575	79	109683	24.259	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	97.040%	
47) 2-Hexanone-d5	10.922	63	83602	43.954	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	87.900%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	209059	24.590	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	98.360%	
66) 1,2-Dichlorobenzene-d4	13.849	152	241799	27.701	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	110.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025789.D
Acq On : 02 May 2023 10:00
Operator : SY/MD
Sample : VW0502SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK493

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:21:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

