




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025793.D
 Acq On : 02 May 2023 12:39
 Operator : SY/MD
 Sample : 02549-06
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN7

Manual IntegrationsAPPROVED

Quant Time: May 03 01:22:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

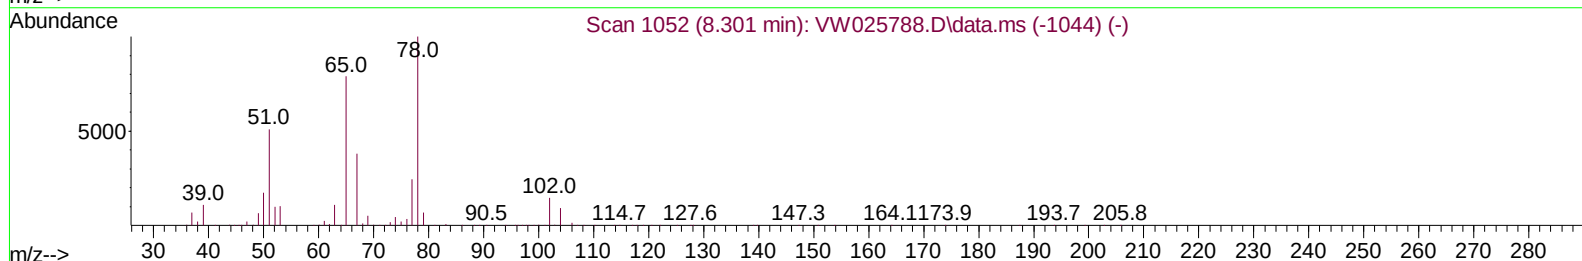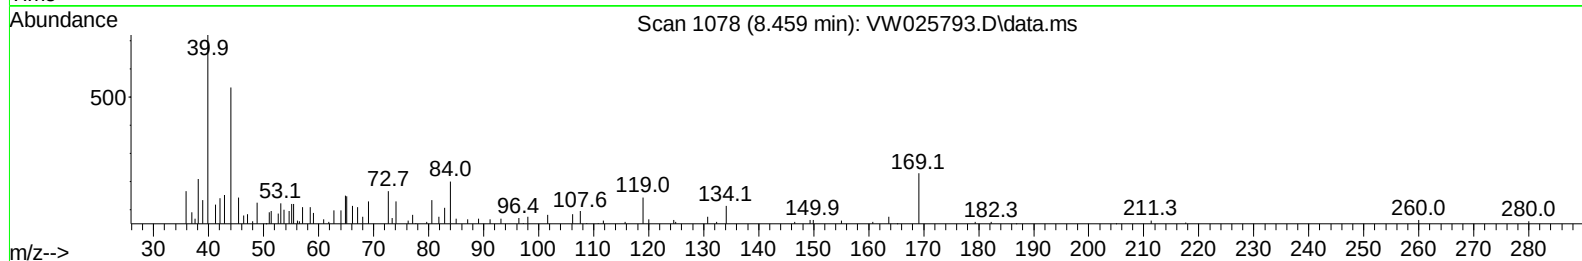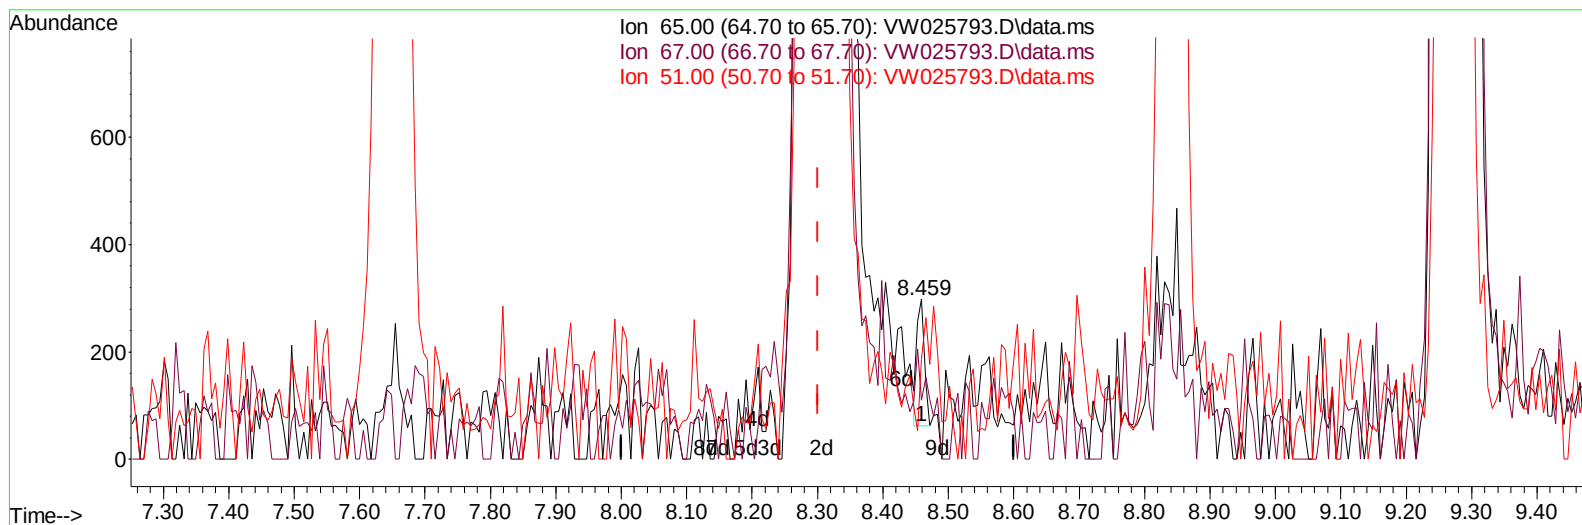

TIC: VW025793.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.459min (+ 0.159) 0.03 ug/L

response 187

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	37.43
51.00	112.30	91.98
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025793.D
 Acq On : 02 May 2023 12:39
 Operator : SY/MD
 Sample : 02549-06
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN7

Manual IntegrationsAPPROVED

Quant Time: May 03 01:22:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

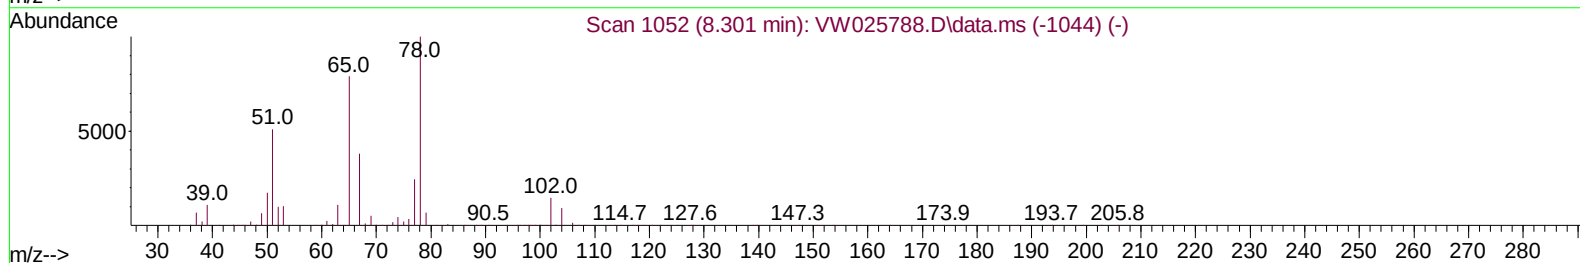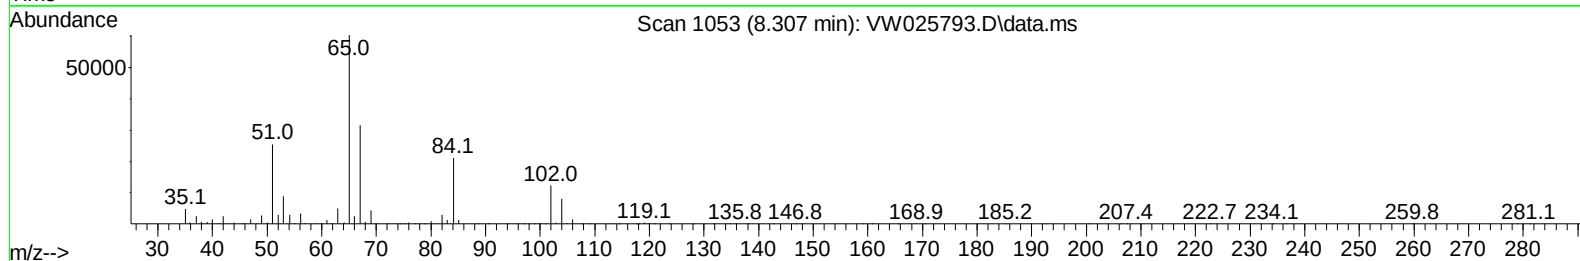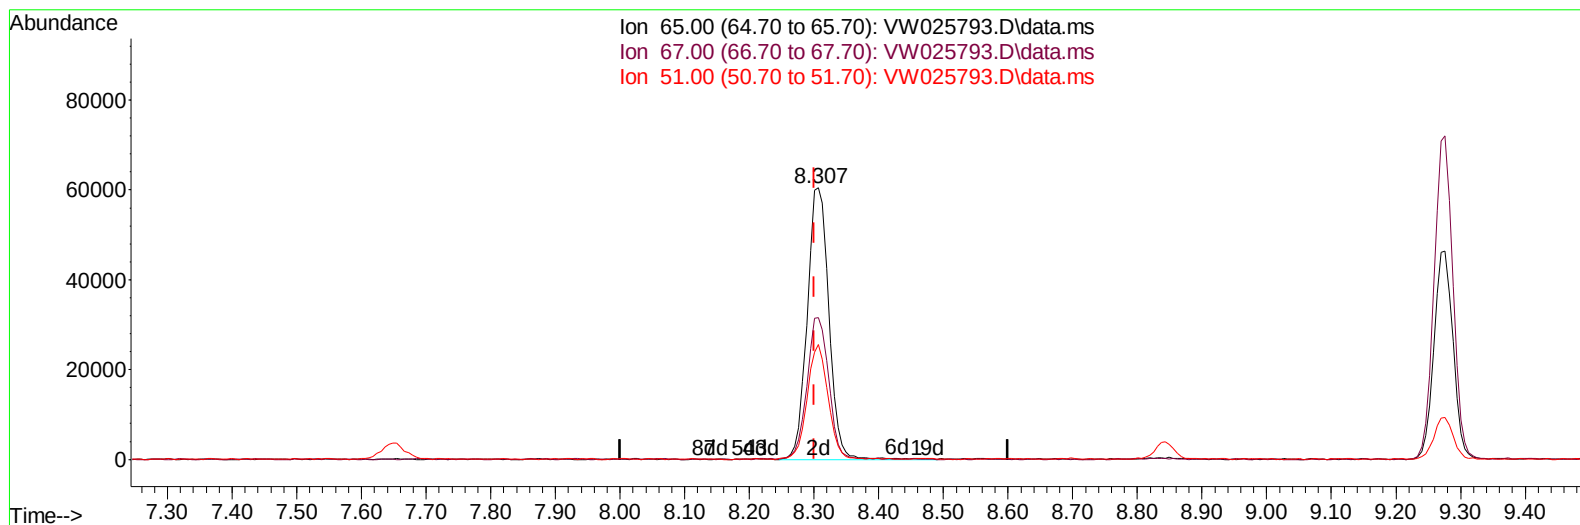

TIC: VW025793.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 24.83 ug/L m

response 140261

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.05#
51.00	112.30	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025793.D
 Acq On : 02 May 2023 12:39
 Operator : SY/MD
 Sample : 02549-06
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN7

Manual IntegrationsAPPROVED

Quant Time: May 03 01:22:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		346496	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		327038	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		144883	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		124490	25.354	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	101.400%	
7) Chloroethane-d5	2.899	69		88827	24.402	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	97.600%	
11) 1,1-Dichloroethene-d2	4.015	65		56312	22.904	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	91.600%	
21) 2-Butanone-d5	7.075	46		90841	55.964	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	111.920%	
24) Chloroform-d	7.655	84		212951	21.314	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	85.240%	
26) 1,2-Dichloroethane-d4	8.307	65		140261m	24.826	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	99.320%	
32) Benzene-d6	8.276	84		441829	20.676	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	82.720%	
36) 1,2-Dichloropropane-d6	9.276	67		146036	21.359	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	85.440%	
41) Toluene-d8	10.325	98		374578	19.657	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	78.640%	
43) trans-1,3-Dichloroprop...	10.575	79		58773	21.206	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	84.840%	
47) 2-Hexanone-d5	10.922	63		58919	50.536	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	101.080%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		134825	25.872	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	103.480%	
66) 1,2-Dichlorobenzene-d4	13.849	152		123672	23.416	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	93.680%	
Target Compounds							
13) Acetone	4.119	43		4439	3.084	ug/L	Qvalue 63

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025793.D
Acq On : 02 May 2023 12:39
Operator : SY/MD
Sample : 02549-06
Misc : 5.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCN7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:22:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

