




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025797.D
 Acq On : 02 May 2023 14:14
 Operator : SY/MD
 Sample : 02549-23
 Misc : 5.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCJ9

Manual IntegrationsAPPROVED

Quant Time: May 03 01:22:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

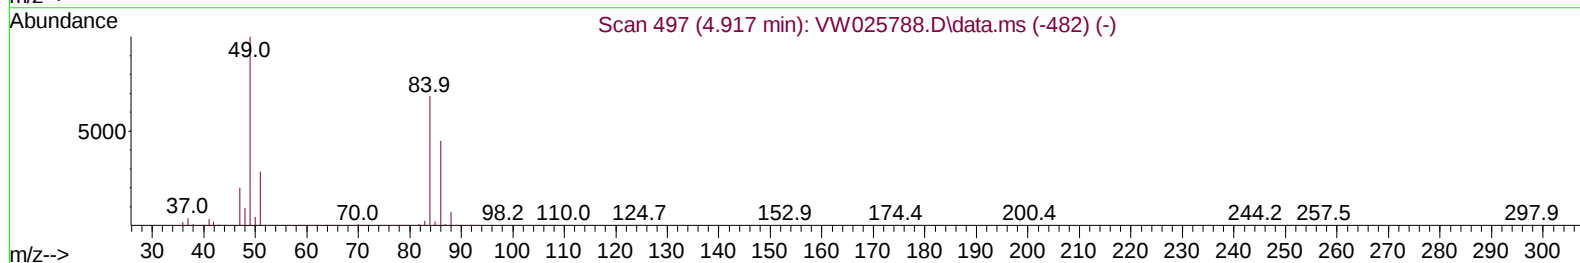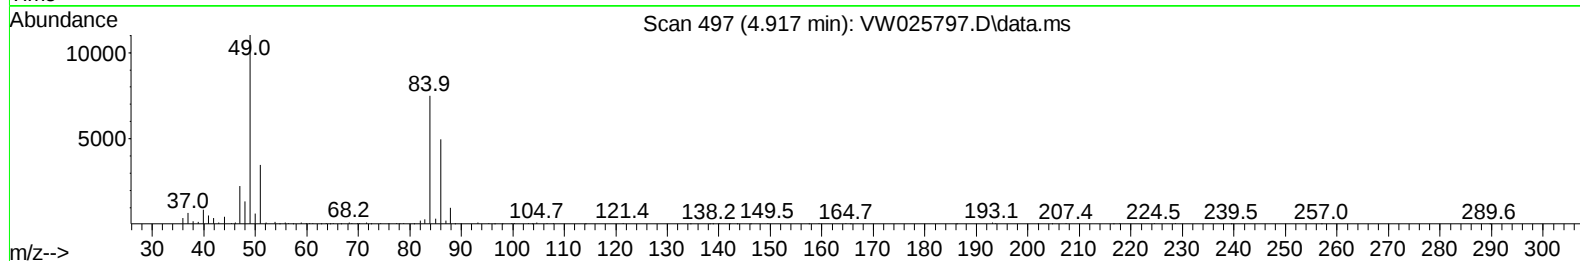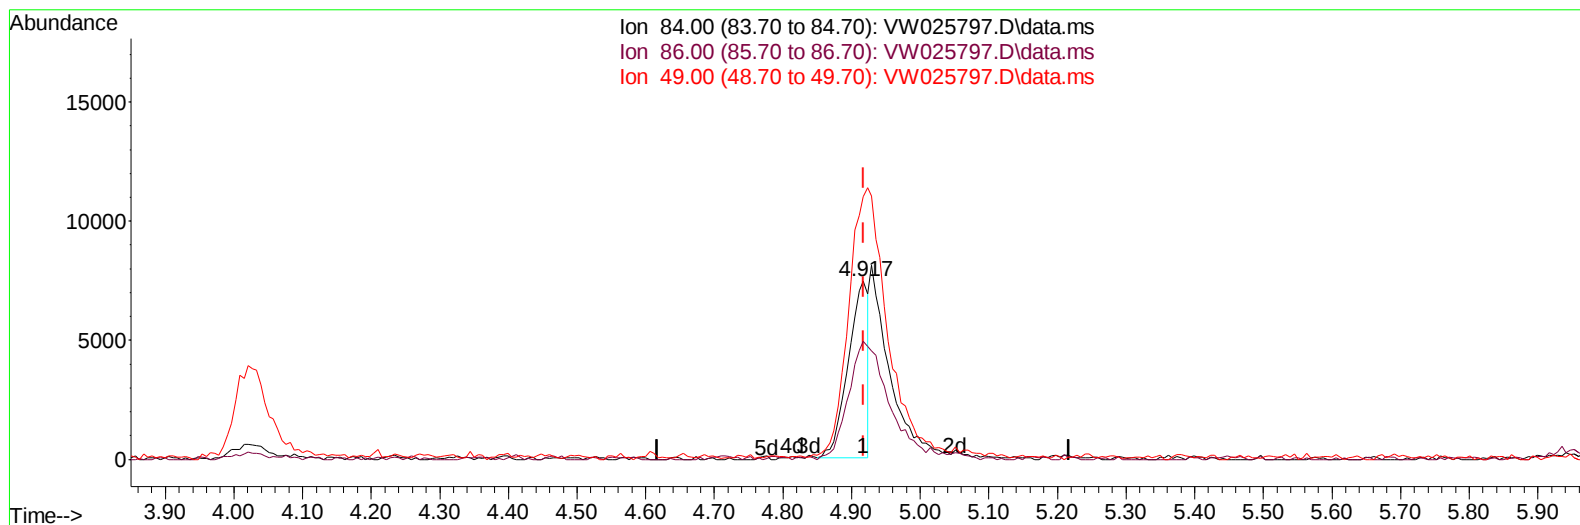

TIC: VW025797.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.000) 0.86 ug/L

response 14963

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	59.60	66.07
49.00	136.20	147.31
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025797.D
 Acq On : 02 May 2023 14:14
 Operator : SY/MD
 Sample : 02549-23
 Misc : 5.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCJ9

Manual IntegrationsAPPROVED

Quant Time: May 03 01:22:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

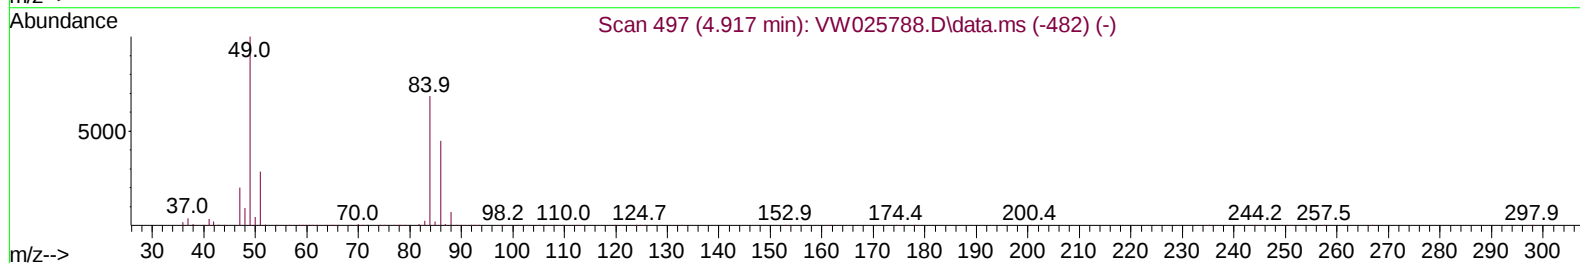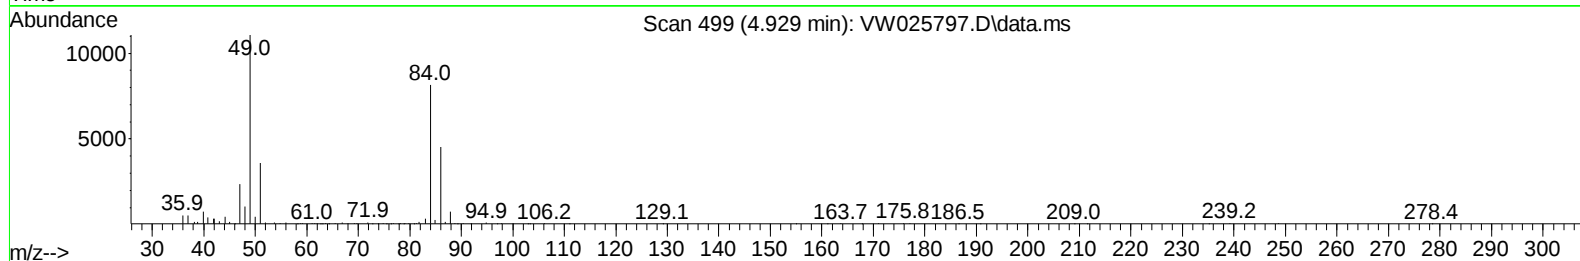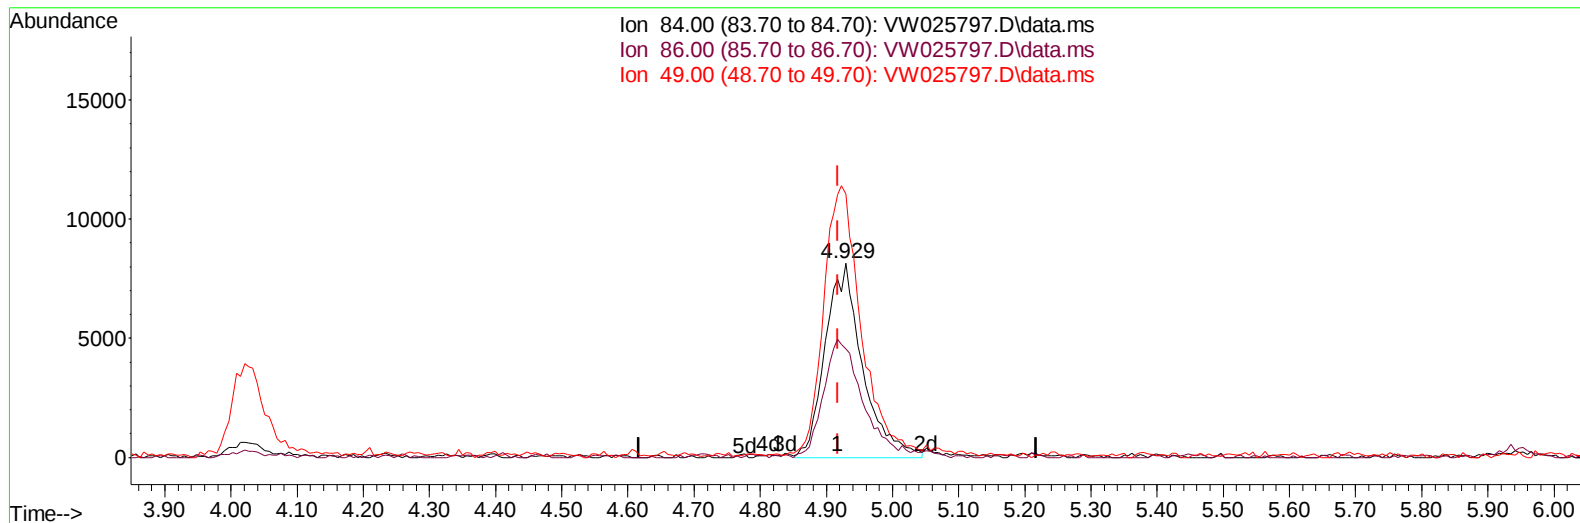

TIC: VW025797.D\data.ms

(16) Methylene chloride (T)

4.929min (+ 0.012) 1.83 ug/L m

response 31884

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	59.60	55.69
49.00	136.20	135.59
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025797.D
 Acq On : 02 May 2023 14:14
 Operator : SY/MD
 Sample : 02549-23
 Misc : 5.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCJ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:22:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	842888	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	784195	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	356169	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	311848	26.109	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	104.440%	
7) Chloroethane-d5	2.899	69	221439	25.007	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	100.040%	
11) 1,1-Dichloroethene-d2	4.021	65	143463	23.987	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	95.960%	
21) 2-Butanone-d5	7.075	46	198731	50.329	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.660%	
24) Chloroform-d	7.648	84	563656	23.191	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.760%	
26) 1,2-Dichloroethane-d4	8.307	65	339069	24.671	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	98.680%	
32) Benzene-d6	8.276	84	1186451	23.154	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	9.270	67	375313	22.892	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.560%	
41) Toluene-d8	10.325	98	1055604	23.102	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	92.400%	
43) trans-1,3-Dichloroprop...	10.575	79	152779	22.989	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.960%	
47) 2-Hexanone-d5	10.922	63	137507	49.186	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.380%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	305162	24.421	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	97.680%	
66) 1,2-Dichlorobenzene-d4	13.848	152	327290	25.208	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.840%	
Target Compounds						
						Qvalue
13) Acetone	4.118	43	210200	60.035	ug/L	99
16) Methylene chloride	4.929	84	31884m	1.834	ug/L	
22) 2-Butanone	7.173	43	19546	4.043	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025797.D
Acq On : 02 May 2023 14:14
Operator : SY/MD
Sample : 02549-23
Misc : 5.68g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCJ9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:22:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

