

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025791.D
 Acq On : 02 May 2023 11:51
 Operator : SY/MD
 Sample : 02549-04
 Misc : 5.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN5

Quant Time: May 03 01:21:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	774161	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	696583	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	326318	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	256117	23.346	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.400%
7) Chloroethane-d5	2.899	69	185518	22.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.240%
11) 1,1-Dichloroethene-d2	4.021	65	120754	21.982	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.920%
21) 2-Butanone-d5	7.075	46	180120	49.665	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.340%
24) Chloroform-d	7.648	84	471393	21.117	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.480%
26) 1,2-Dichloroethane-d4	8.307	65	288298	22.839	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.360%
32) Benzene-d6	8.276	84	987252	21.690	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.760%
36) 1,2-Dichloropropane-d6	9.276	67	316166	21.710	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.840%
41) Toluene-d8	10.325	98	877809	21.628	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.520%
43) trans-1,3-Dichloroprop...	10.575	79	130322	22.077	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.320%
47) 2-Hexanone-d5	10.922	63	122327	49.260	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.520%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	267695	24.117	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	281177	23.637	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.560%
Target Compounds					Qvalue	
13) Acetone	4.131	43	12223	3.801	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025791.D
Acq On : 02 May 2023 11:51
Operator : SY/MD
Sample : 02549-04
Misc : 5.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCN5

Quant Time: May 03 01:21:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

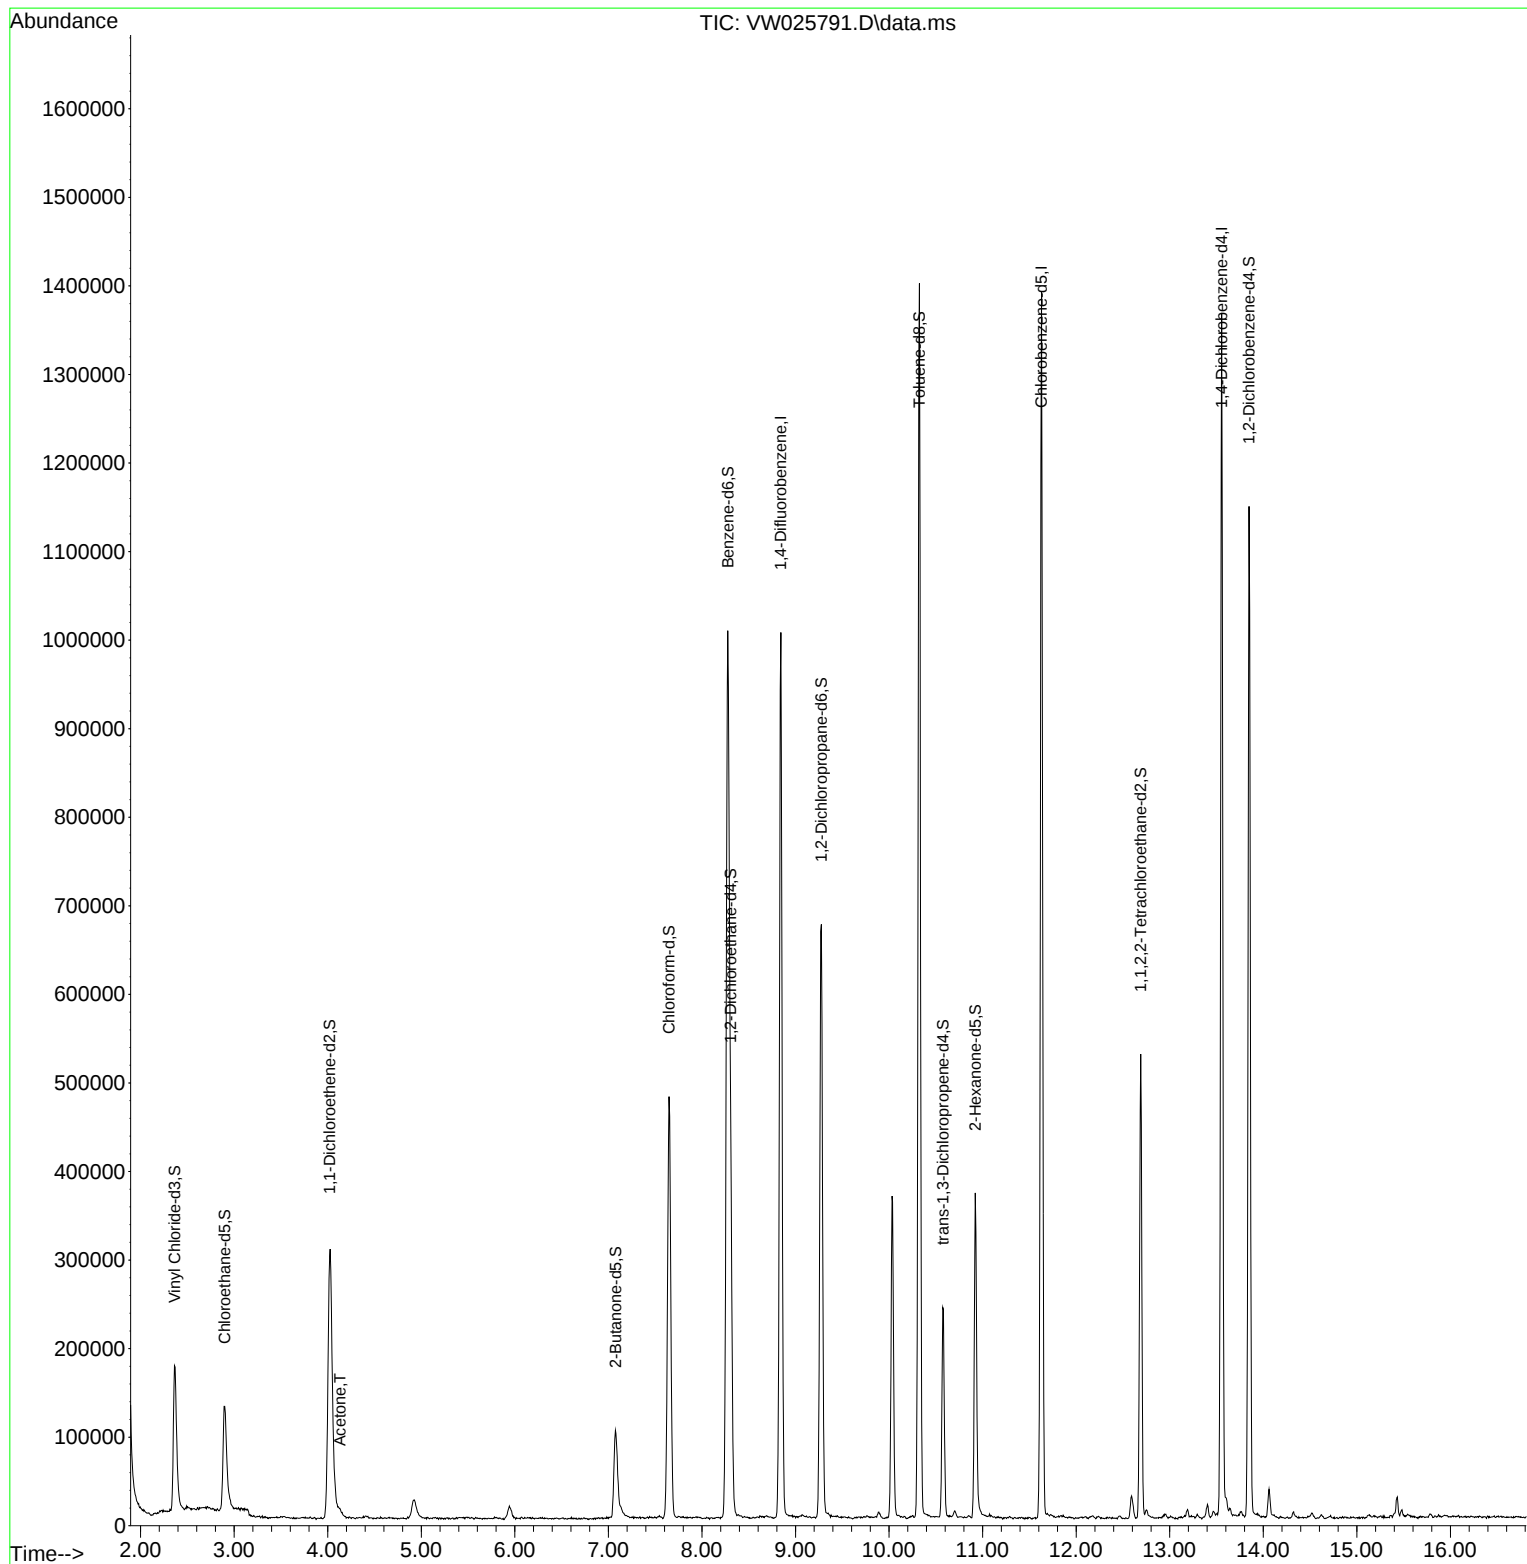

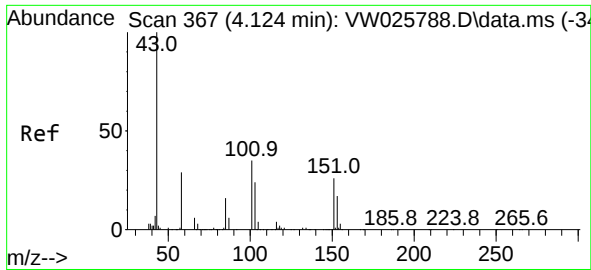

#13
 Acetone
 Concen: 3.801 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW025791.D
 Acq: 02 May 2023 11:51

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN5

Tgt Ion: 43 Resp: 12223
 Ion Ratio Lower Upper
 43 100
 58 32.3 0.0 58.2

