

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025792.D
 Acq On : 02 May 2023 12:15
 Operator : SY/MD
 Sample : 02549-05
 Misc : 5.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN6

Quant Time: May 03 01:21:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	332024	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	315017	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	139841	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.357	65	132602	28.183	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.720%	
7) Chloroethane-d5		2.899	69	93810	26.894	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.560%	
11) 1,1-Dichloroethene-d2		4.021	65	61632	26.160	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	104.640%	
21) 2-Butanone-d5		7.075	46	84879	54.570	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.140%	
24) Chloroform-d		7.648	84	225400	23.543	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.160%	
26) 1,2-Dichloroethane-d4		8.307	65	139793	25.821	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.280%	
32) Benzene-d6		8.276	84	466000	22.639	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.560%	
36) 1,2-Dichloropropane-d6		9.276	67	154168	23.409	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.640%	
41) Toluene-d8		10.325	98	394632	21.500	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.000%	
43) trans-1,3-Dichloroprop...		10.581	79	60450	22.644	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.560%	
47) 2-Hexanone-d5		10.922	63	53859	47.959	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.920%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	130620	26.022	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.080%	
66) 1,2-Dichlorobenzene-d4		13.848	152	126571	24.829	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.320%	
Target Compounds							
13) Acetone		4.131	43	7188	5.212	ug/L	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025792.D
Acq On : 02 May 2023 12:15
Operator : SY/MD
Sample : 02549-05
Misc : 5.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCN6

Quant Time: May 03 01:21:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

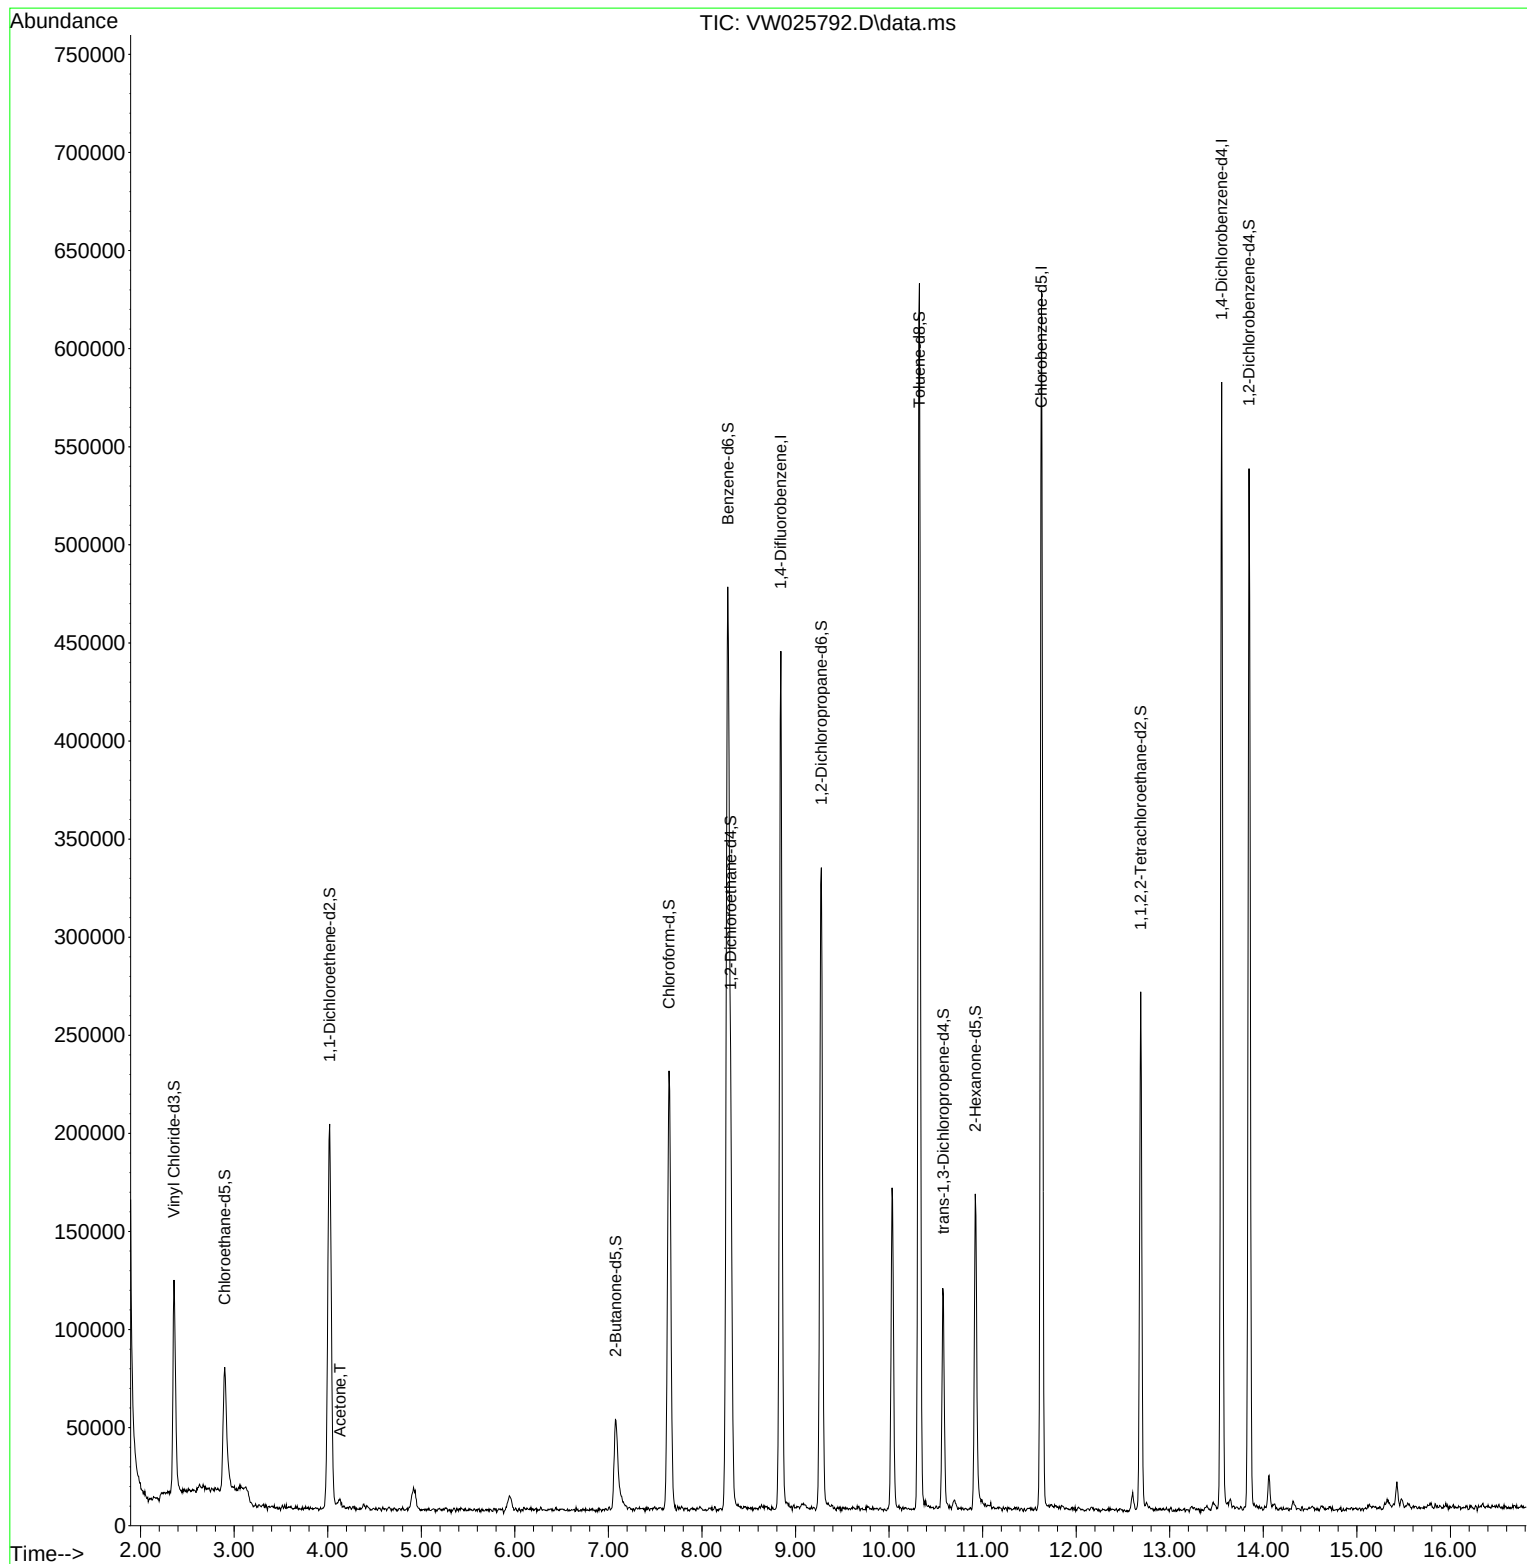

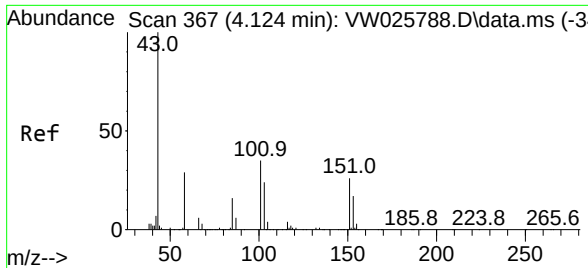

#13
 Acetone
 Concen: 5.212 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW025792.D
 Acq: 02 May 2023 12:15

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN6

Tgt Ion: 43 Resp: 7188
 Ion Ratio Lower Upper
 43 100
 58 19.3 0.0 58.2

