

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025793.D
 Acq On : 02 May 2023 12:39
 Operator : SY/MD
 Sample : 02549-06
 Misc : 5.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN7

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:22:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	346496	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	327038	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	144883	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	124490	25.354	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 101.400%			
7) Chloroethane-d5	2.899	69	88827	24.402	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 97.600%			
11) 1,1-Dichloroethene-d2	4.015	65	56312	22.904	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 91.600%			
21) 2-Butanone-d5	7.075	46	90841	55.964	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 111.920%			
24) Chloroform-d	7.655	84	212951	21.314	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 85.240%			
26) 1,2-Dichloroethane-d4	8.307	65	140261m	24.826	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 99.320%			
32) Benzene-d6	8.276	84	441829	20.676	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 82.720%			
36) 1,2-Dichloropropane-d6	9.276	67	146036	21.359	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 85.440%			
41) Toluene-d8	10.325	98	374578	19.657	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 78.640%			
43) trans-1,3-Dichloroprop...	10.575	79	58773	21.206	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 84.840%			
47) 2-Hexanone-d5	10.922	63	58919	50.536	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 101.080%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	134825	25.872	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 103.480%			
66) 1,2-Dichlorobenzene-d4	13.849	152	123672	23.416	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 93.680%			
Target Compounds					Qvalue	
13) Acetone	4.119	43	4439	3.084	ug/L	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025793.D
Acq On : 02 May 2023 12:39
Operator : SY/MD
Sample : 02549-06
Misc : 5.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DCCN7

Quant Time: May 03 01:22:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/03/2023
Supervised By :Mahesh Dadoda 05/03/2023

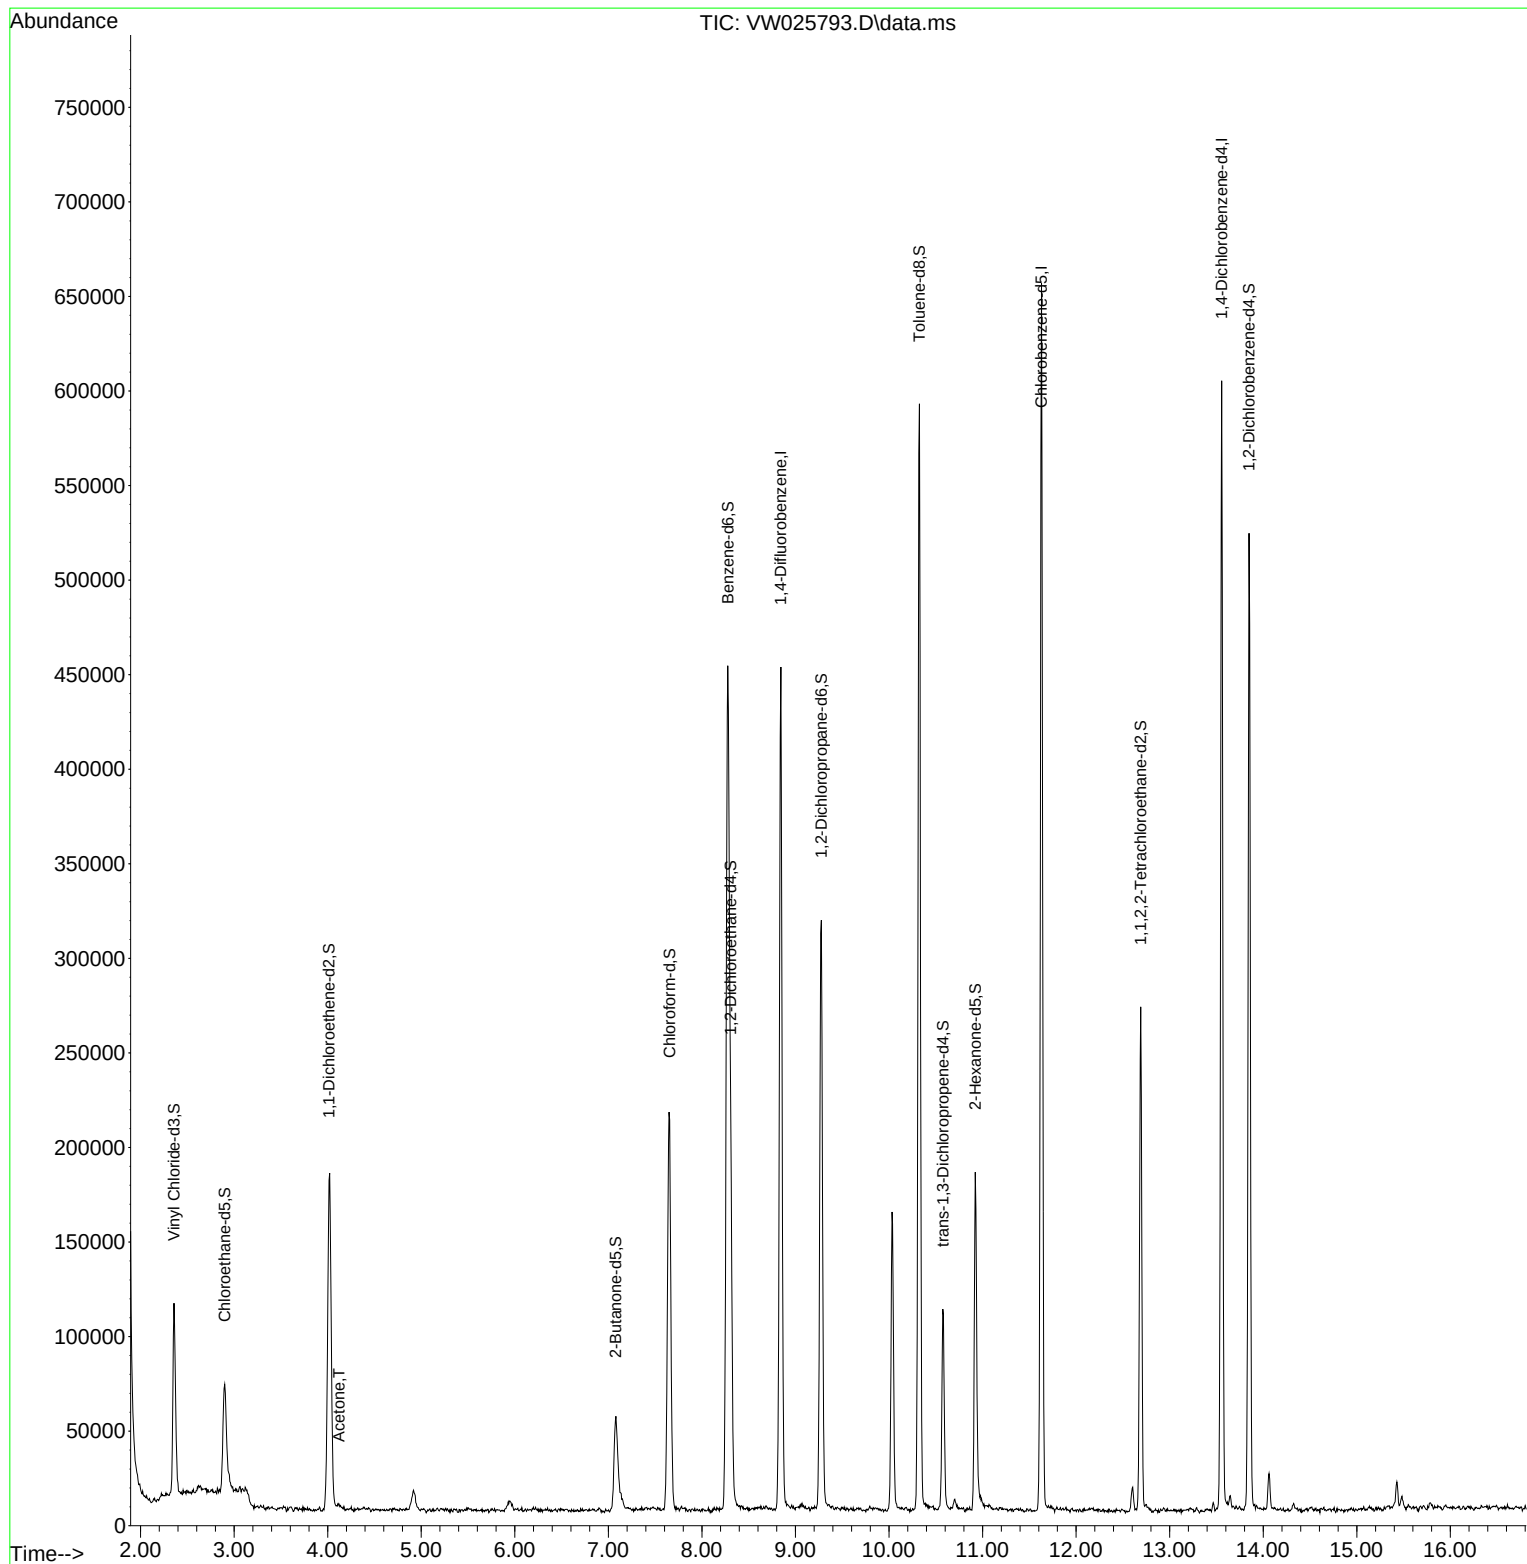

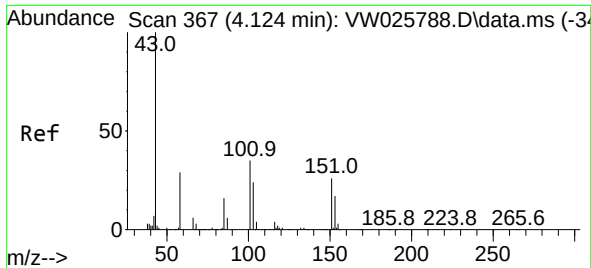

#13
 Acetone
 Concen: 3.084 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025793.D
 Acq: 02 May 2023 12:39

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN7

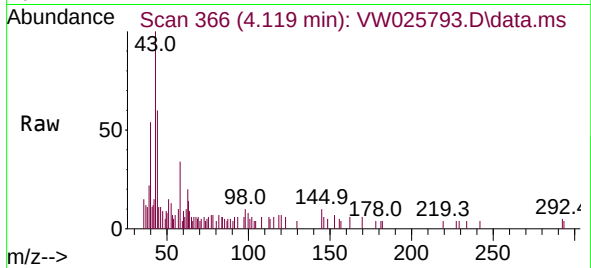

Tgt Ion: 43 Resp: 4439
 Ion Ratio Lower Upper
 43 100
 58 9.4 0.0 58.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

