

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025796.D
 Acq On : 02 May 2023 13:50
 Operator : SY/MD
 Sample : 02549-03
 Misc : 5.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCN4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:22:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	846741	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	765417	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	358146	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	240285	20.026	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.120%		
7) Chloroethane-d5	2.905	69	171698	19.301	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.200%		
11) 1,1-Dichloroethene-d2	4.027	65	109002	18.142	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	72.560%		
21) 2-Butanone-d5	7.075	46	191443	48.263	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.520%		
24) Chloroform-d	7.648	84	441488	18.082	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	72.320%		
26) 1,2-Dichloroethane-d4	8.307	65	278623m	20.180	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.720%		
32) Benzene-d6	8.276	84	914969	18.294	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	73.160%		
36) 1,2-Dichloropropane-d6	9.270	67	301007	18.810	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	75.240%		
41) Toluene-d8	10.325	98	806274	18.079	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	72.320%		
43) trans-1,3-Dichloroprop...	10.575	79	125092	19.285	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.120%		
47) 2-Hexanone-d5	10.922	63	131238	48.096	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.200%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	270214	22.155	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	88.600%		
66) 1,2-Dichlorobenzene-d4	13.848	152	261669	20.042	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	80.160%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	128303	36.478	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025796.D
Acq On : 02 May 2023 13:50
Operator : SY/MD
Sample : 02549-03
Misc : 5.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DCCN4

Quant Time: May 03 01:22:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
Supervised By :Mahesh Dadoda 05/03/2023

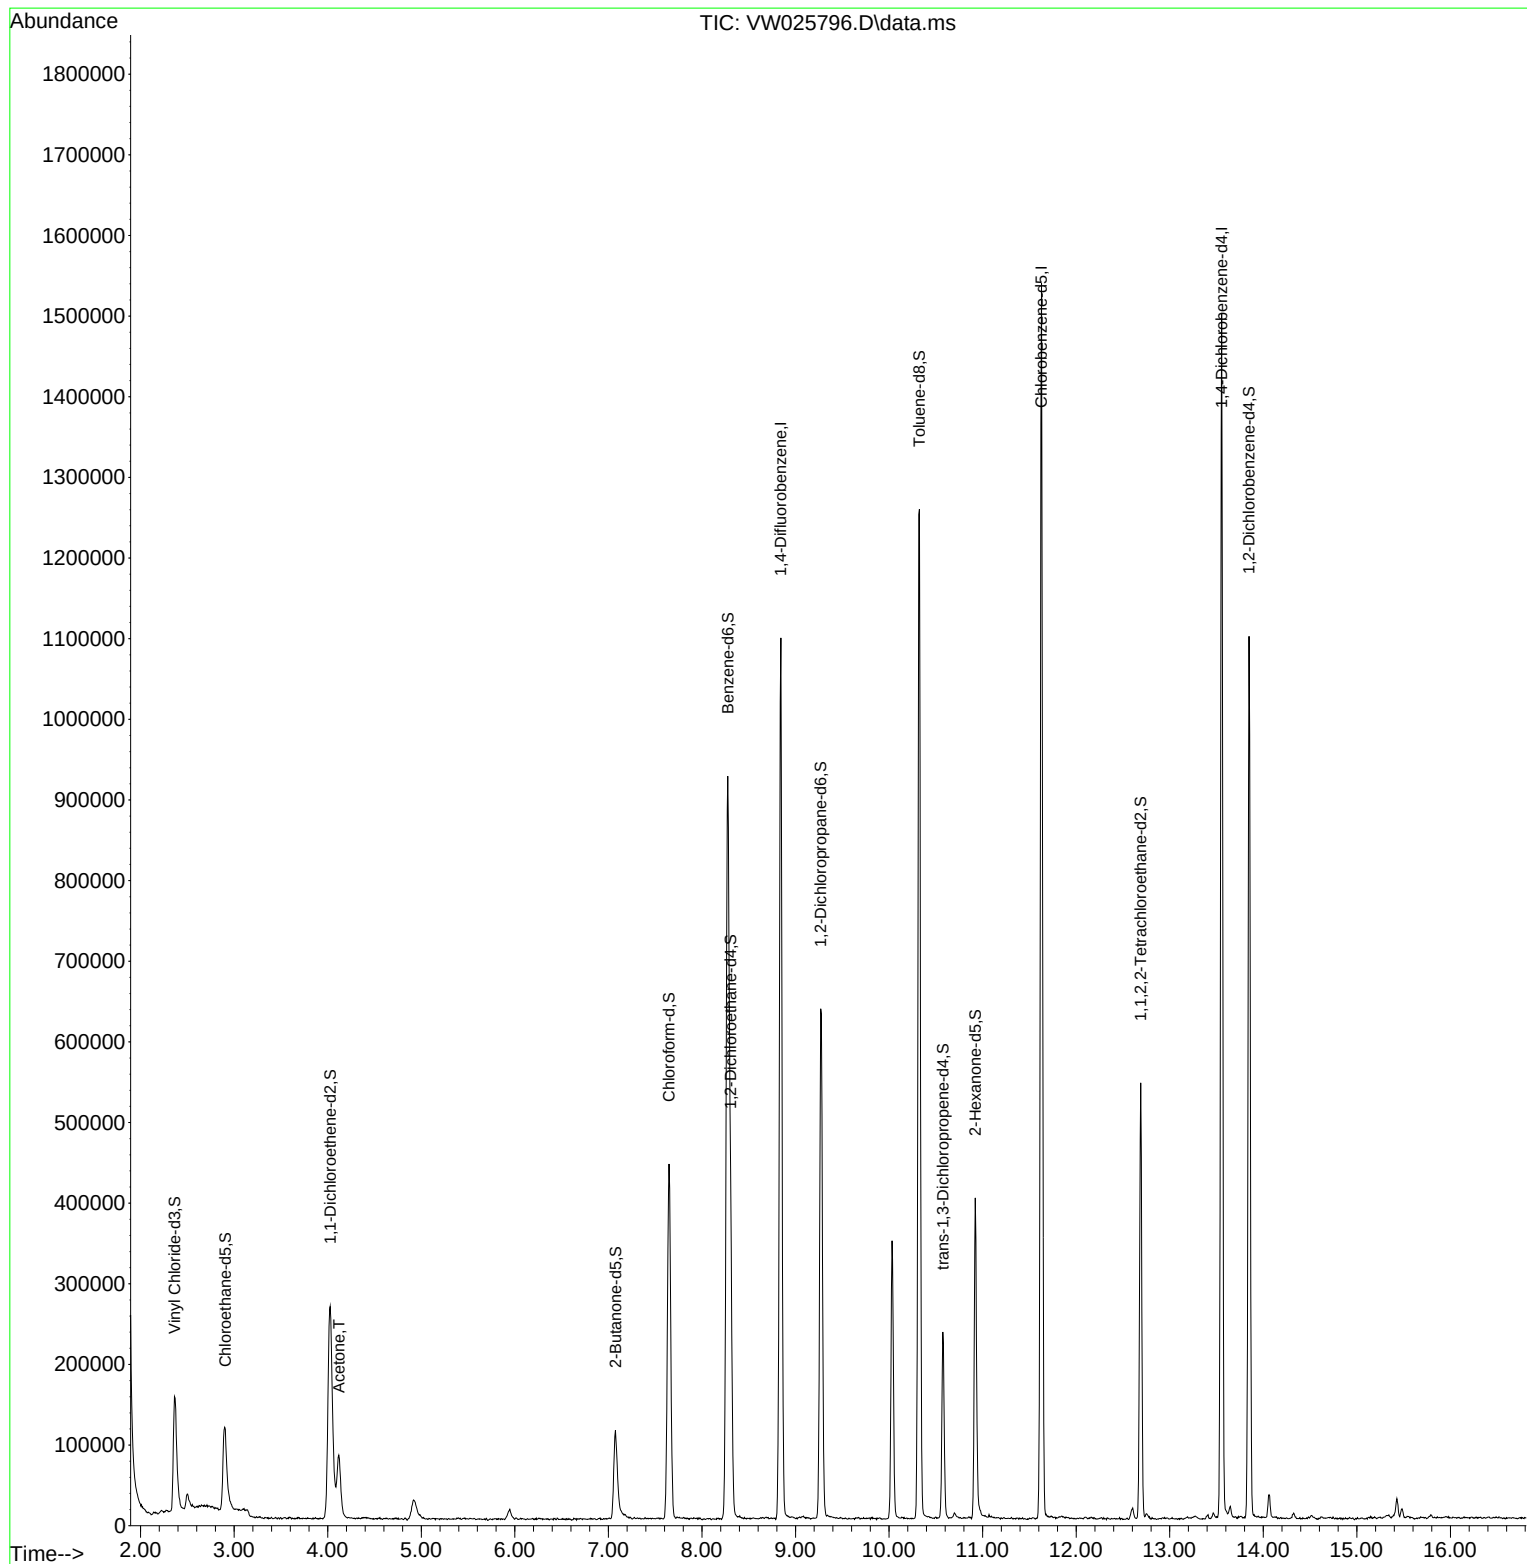

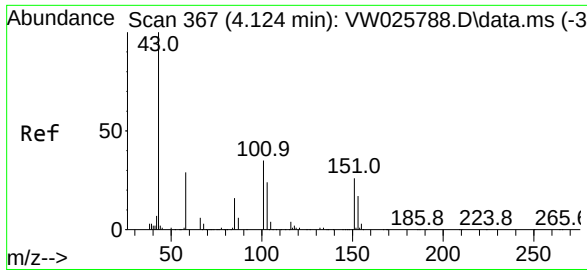

#13

Acetone

Concen: 36.478 ug/L

RT: 4.118 min Scan# 30

Delta R.T. -0.006 min

Lab File: VW025796.D

Acq: 02 May 2023 13:50

Instrument :

MSVOA_W

ClientSampleId :

DCCN4

Tgt Ion: 43 Resp: 12830

Ion Ratio Lower Upper

43 100

58 29.6 0.0 58.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023

Supervised By :Mahesh Dadoda 05/03/2023

