

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025801.D
 Acq On : 02 May 2023 15:50
 Operator : SY/MD
 Sample : VIBLK450
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK450

Quant Time: May 03 01:23:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	646698	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	584174	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	268702	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	216068	23.578	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.320%		
7) Chloroethane-d5	2.899	69	156004	22.962	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.840%		
11) 1,1-Dichloroethene-d2	4.027	65	99815	21.752	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	87.000%		
21) 2-Butanone-d5	7.075	46	121072	39.964	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.920%		
24) Chloroform-d	7.648	84	393582	21.106	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.440%		
26) 1,2-Dichloroethane-d4	8.307	65	227554	21.580	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	86.320%		
32) Benzene-d6	8.276	84	833688	21.841	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.360%		
36) 1,2-Dichloropropane-d6	9.270	67	263059	21.539	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.160%		
41) Toluene-d8	10.319	98	726418	21.341	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.360%		
43) trans-1,3-Dichloroprop...	10.575	79	98895	19.977	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.920%		
47) 2-Hexanone-d5	10.922	63	81186	38.984	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.960%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	196044	21.061	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	84.240%		
66) 1,2-Dichlorobenzene-d4	13.848	152	222732	22.739	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.960%		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	25543	1.915	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025801.D
Acq On : 02 May 2023 15:50
Operator : SY/MD
Sample : VIBLK450
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK450

Quant Time: May 03 01:23:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

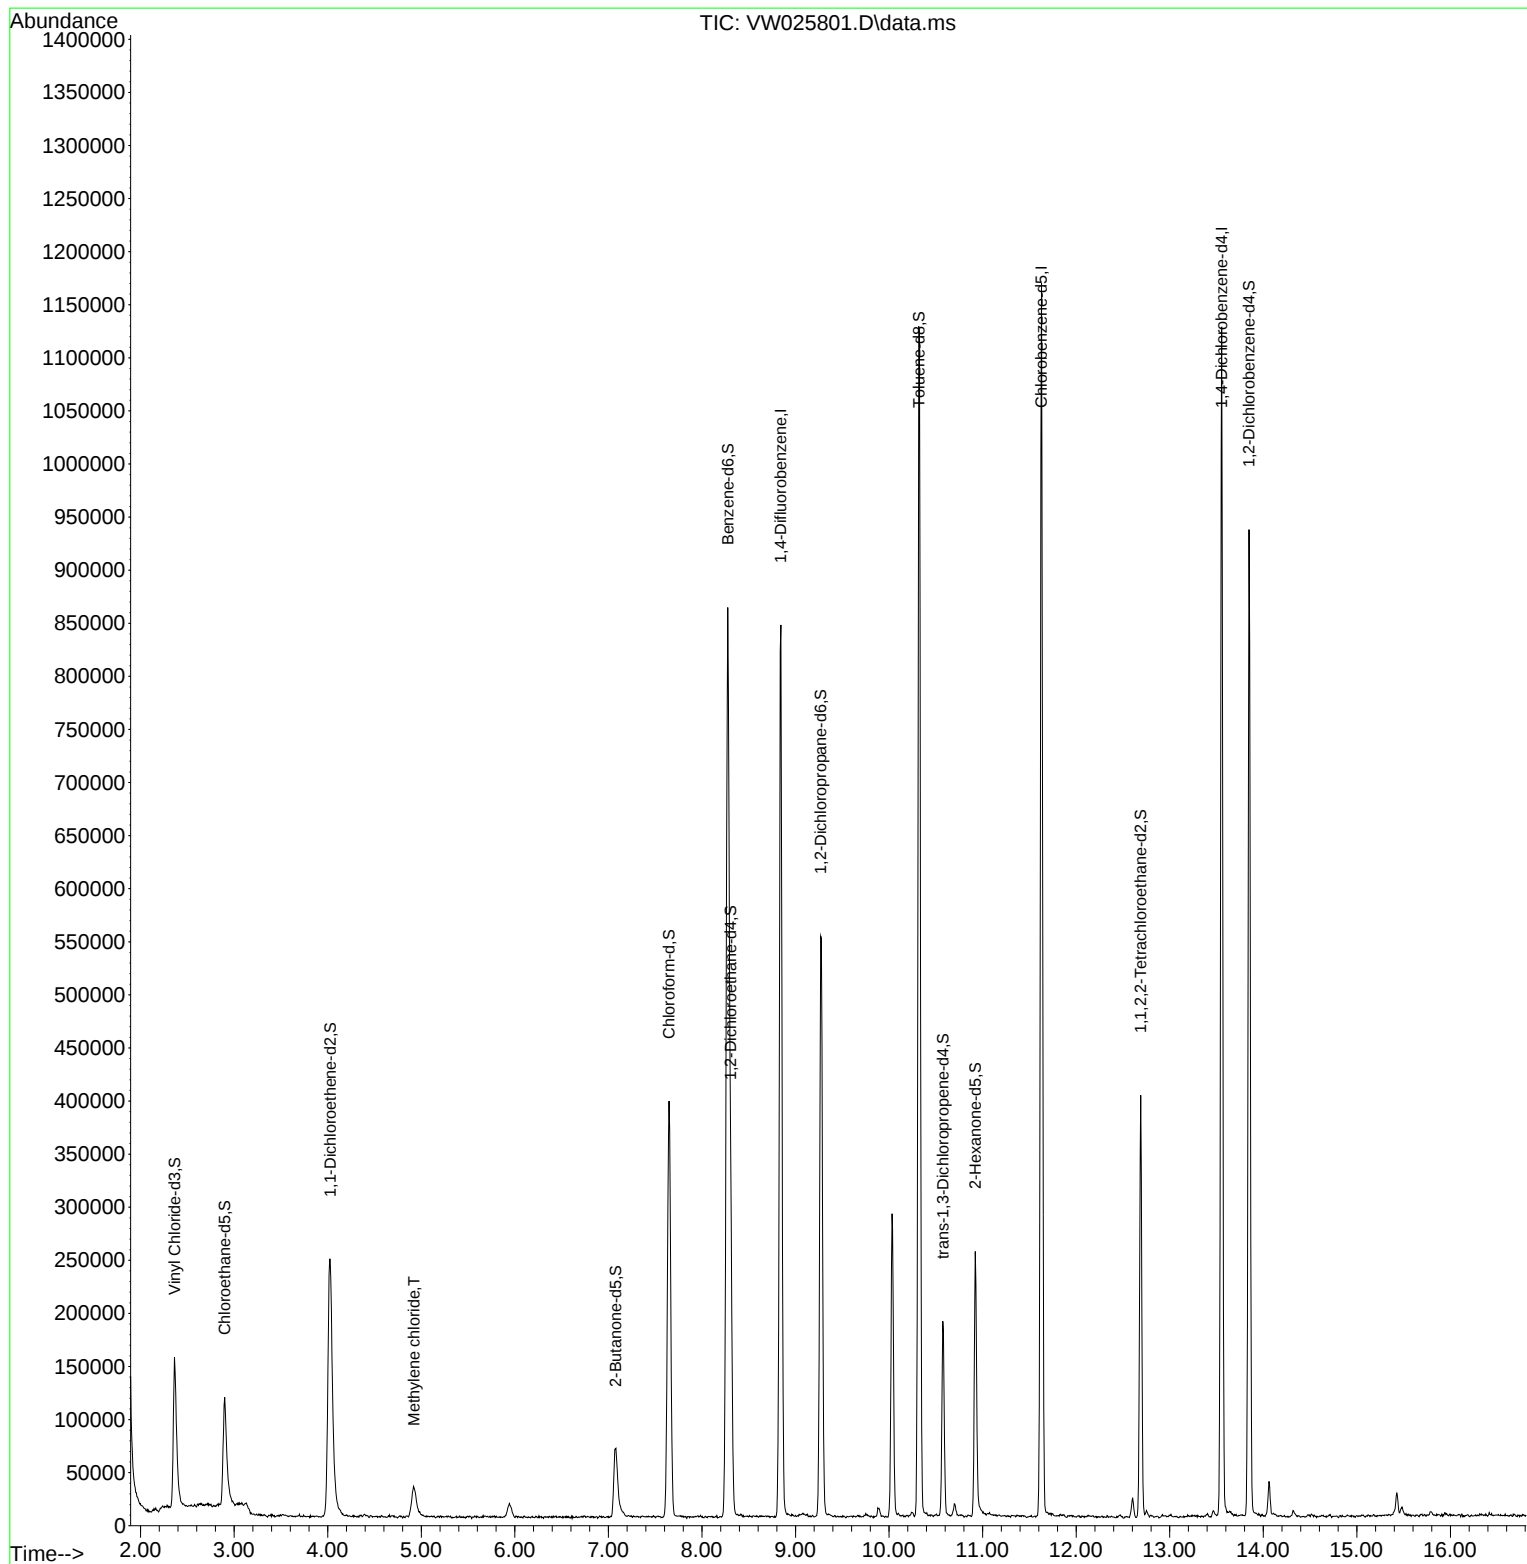

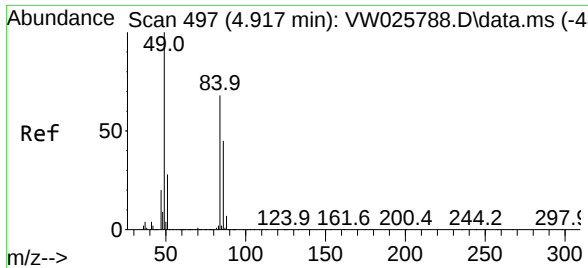

#16
Methylene chloride
Concen: 1.915 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW025801.D
Acq: 02 May 2023 15:50

Instrument :
MSVOA_W
ClientSampleId :
VIBLK450

Tgt Ion:	84	Resp:	25543
Ion	Ratio	Lower	Upper
84	100		
86	56.3	41.7	77.5
49	129.1	95.3	177.1

