

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
 Data File : VW025807.D
 Acq On : 02 May 2023 18:14
 Operator : SY/MD
 Sample : 02549-24
 Misc : 6.16g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCK0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023
 Supervised By :Mahesh Dadoda 05/03/2023

Quant Time: May 03 01:24:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 03 01:20:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	847153	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	754037	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	344206	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	278883	23.231	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.920%		
7) Chloroethane-d5	2.893	69	203914	22.912	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.640%		
11) 1,1-Dichloroethene-d2	4.027	65	134377	22.354	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	89.400%		
21) 2-Butanone-d5	7.075	46	201683	50.819	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.640%		
24) Chloroform-d	7.648	84	544753	22.301	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.200%		
26) 1,2-Dichloroethane-d4	8.307	65	337310m	24.419	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.680%		
32) Benzene-d6	8.270	84	1124079	22.815	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	91.240%		
36) 1,2-Dichloropropane-d6	9.270	67	368320	23.364	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.440%		
41) Toluene-d8	10.319	98	1009533	22.978	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	91.920%		
43) trans-1,3-Dichloroprop...	10.575	79	147924	23.149	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	92.600%		
47) 2-Hexanone-d5	10.922	63	137813	51.268	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.540%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	306171	25.482	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.920%		
66) 1,2-Dichlorobenzene-d4	13.849	152	324284	25.844	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.360%		
Target Compounds					Qvalue	
13) Acetone	4.119	43	161559	45.911	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050223\
Data File : VW025807.D
Acq On : 02 May 2023 18:14
Operator : SY/MD
Sample : 02549-24
Misc : 6.16g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DCKK0

Quant Time: May 03 01:24:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 03 01:20:37 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/03/2023
Supervised By : Mahesh Dadoda 05/03/2023

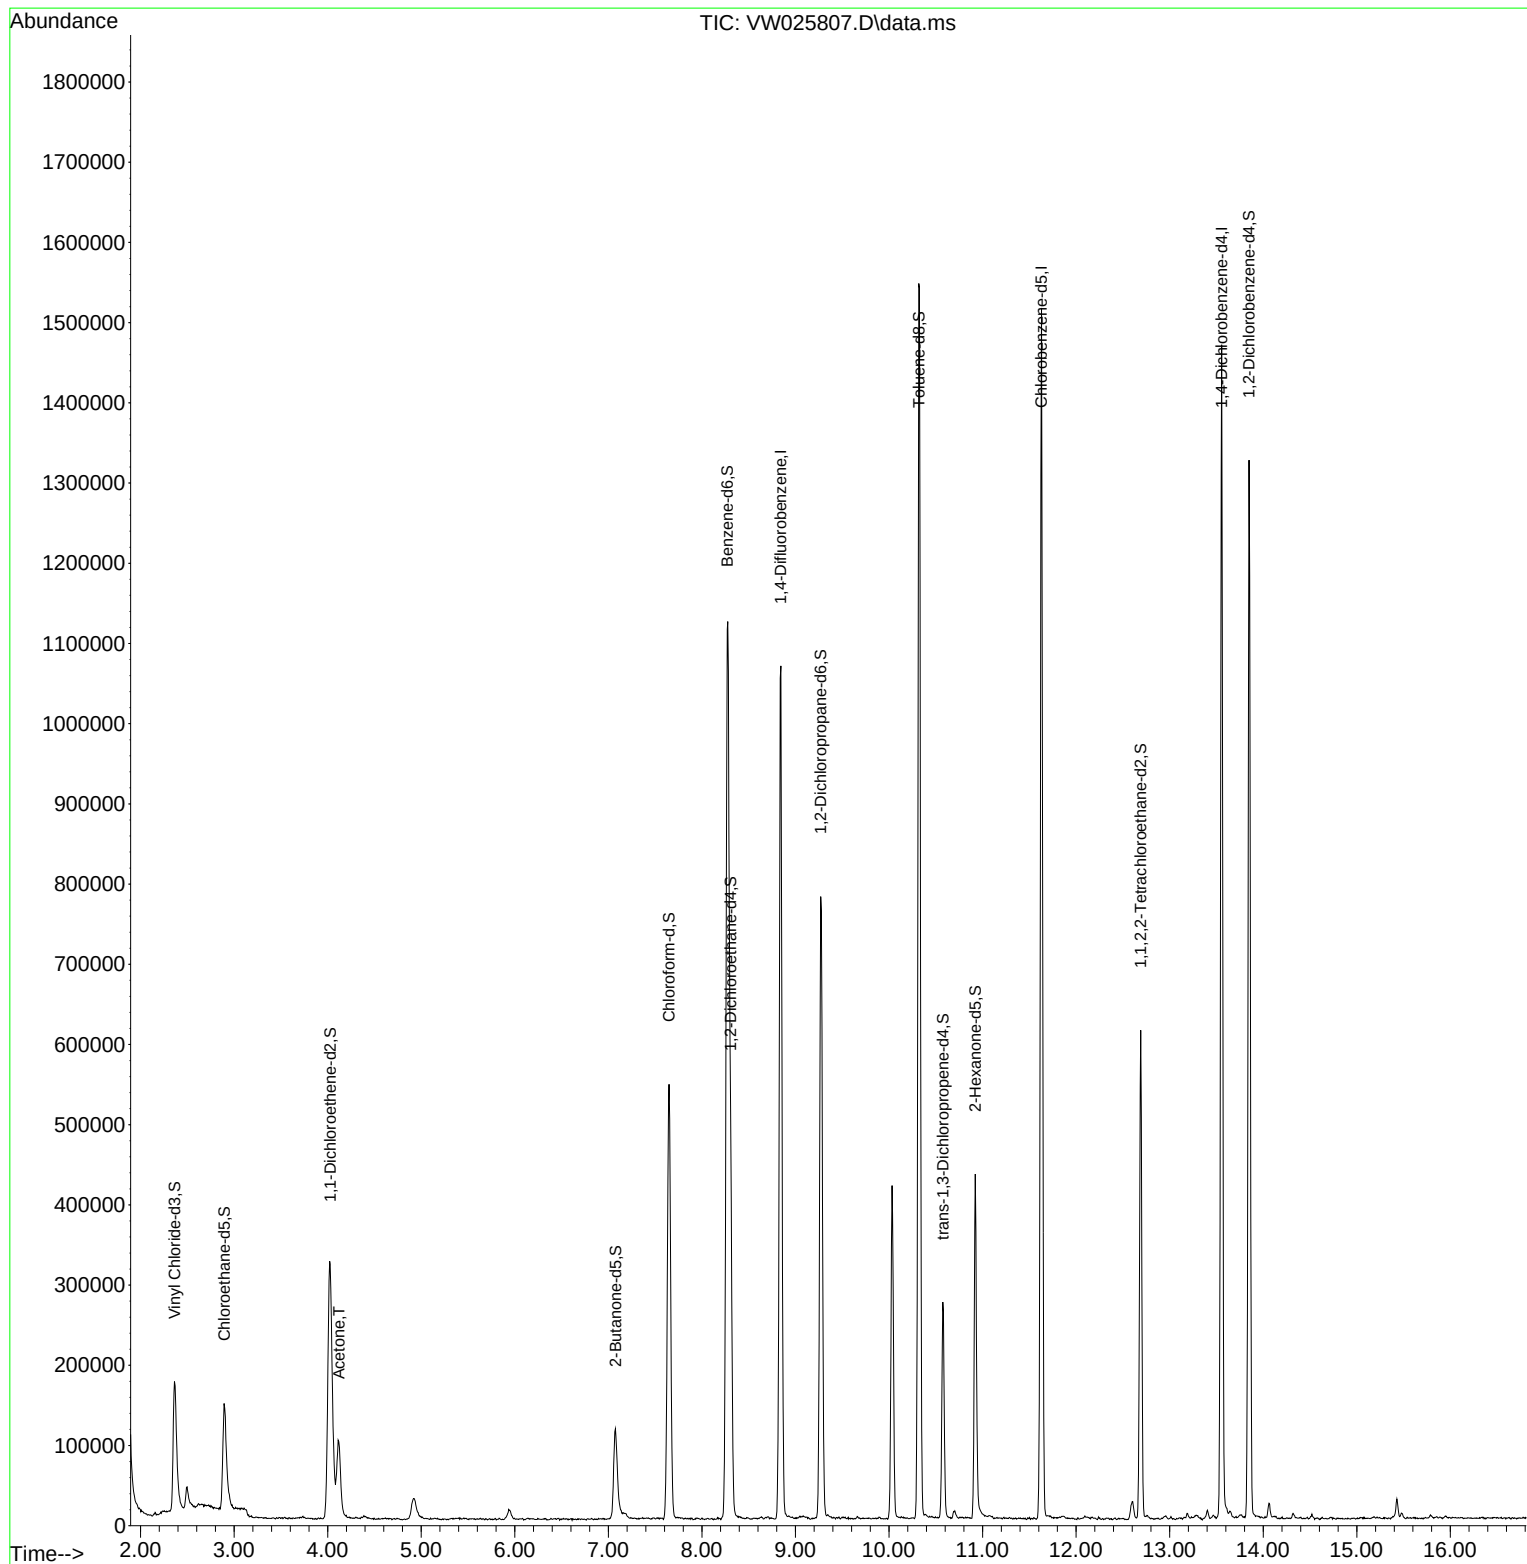

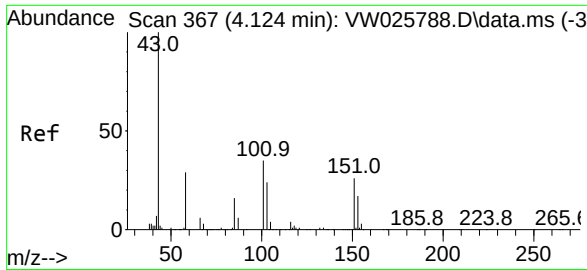

#13

Acetone

Concen: 45.911 ug/L

RT: 4.119 min Scan# 30

Delta R.T. -0.006 min

Lab File: VW025807.D

Acq: 02 May 2023 18:14

Instrument :

MSVOA_W

ClientSampleId :

DCCK0

Tgt Ion: 43 Resp: 16155

Ion Ratio Lower Upper

43 100

58 29.9 0.0 58.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 05/03/2023

Supervised By :Mahesh Dadoda 05/03/2023

