

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050224\
 Data File : VW028577.D
 Acq On : 02 May 2024 17:21
 Operator : SY/MD
 Sample : P2349-02
 Misc : 5.71g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 03 04:10:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 03 04:07:09 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	439500	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	402501	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	184069	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	144571	17.323	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.280%
7) Chloroethane-d5	2.899	69	113619	17.780	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.120%
11) 1,1-Dichloroethene-d2	4.021	65	61613	17.670	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.680%
21) 2-Butanone-d5	7.075	46	70411	32.338	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.680%
24) Chloroform-d	7.648	84	251948	18.346	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.400%
26) 1,2-Dichloroethane-d4	8.380	65	277	0.035	ug/L	0.07
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.276	84	500187	18.626	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.520%
36) 1,2-Dichloropropane-d6	9.270	67	152443	18.865	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.440%
41) Toluene-d8	10.324	98	451815	18.998	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.000%
43) trans-1,3-Dichloroprop...	10.574	79	60931	18.743	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.960%
47) 2-Hexanone-d5	10.922	63	48531	34.821	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	119340	17.612	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	70.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	143330	20.430	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.720%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	5597	0.574	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050224\
Data File : VW028577.D
Acq On : 02 May 2024 17:21
Operator : SY/MD
Sample : P2349-02
Misc : 5.71g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 03 04:10:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 03 04:07:09 2024
Response via : Initial Calibration

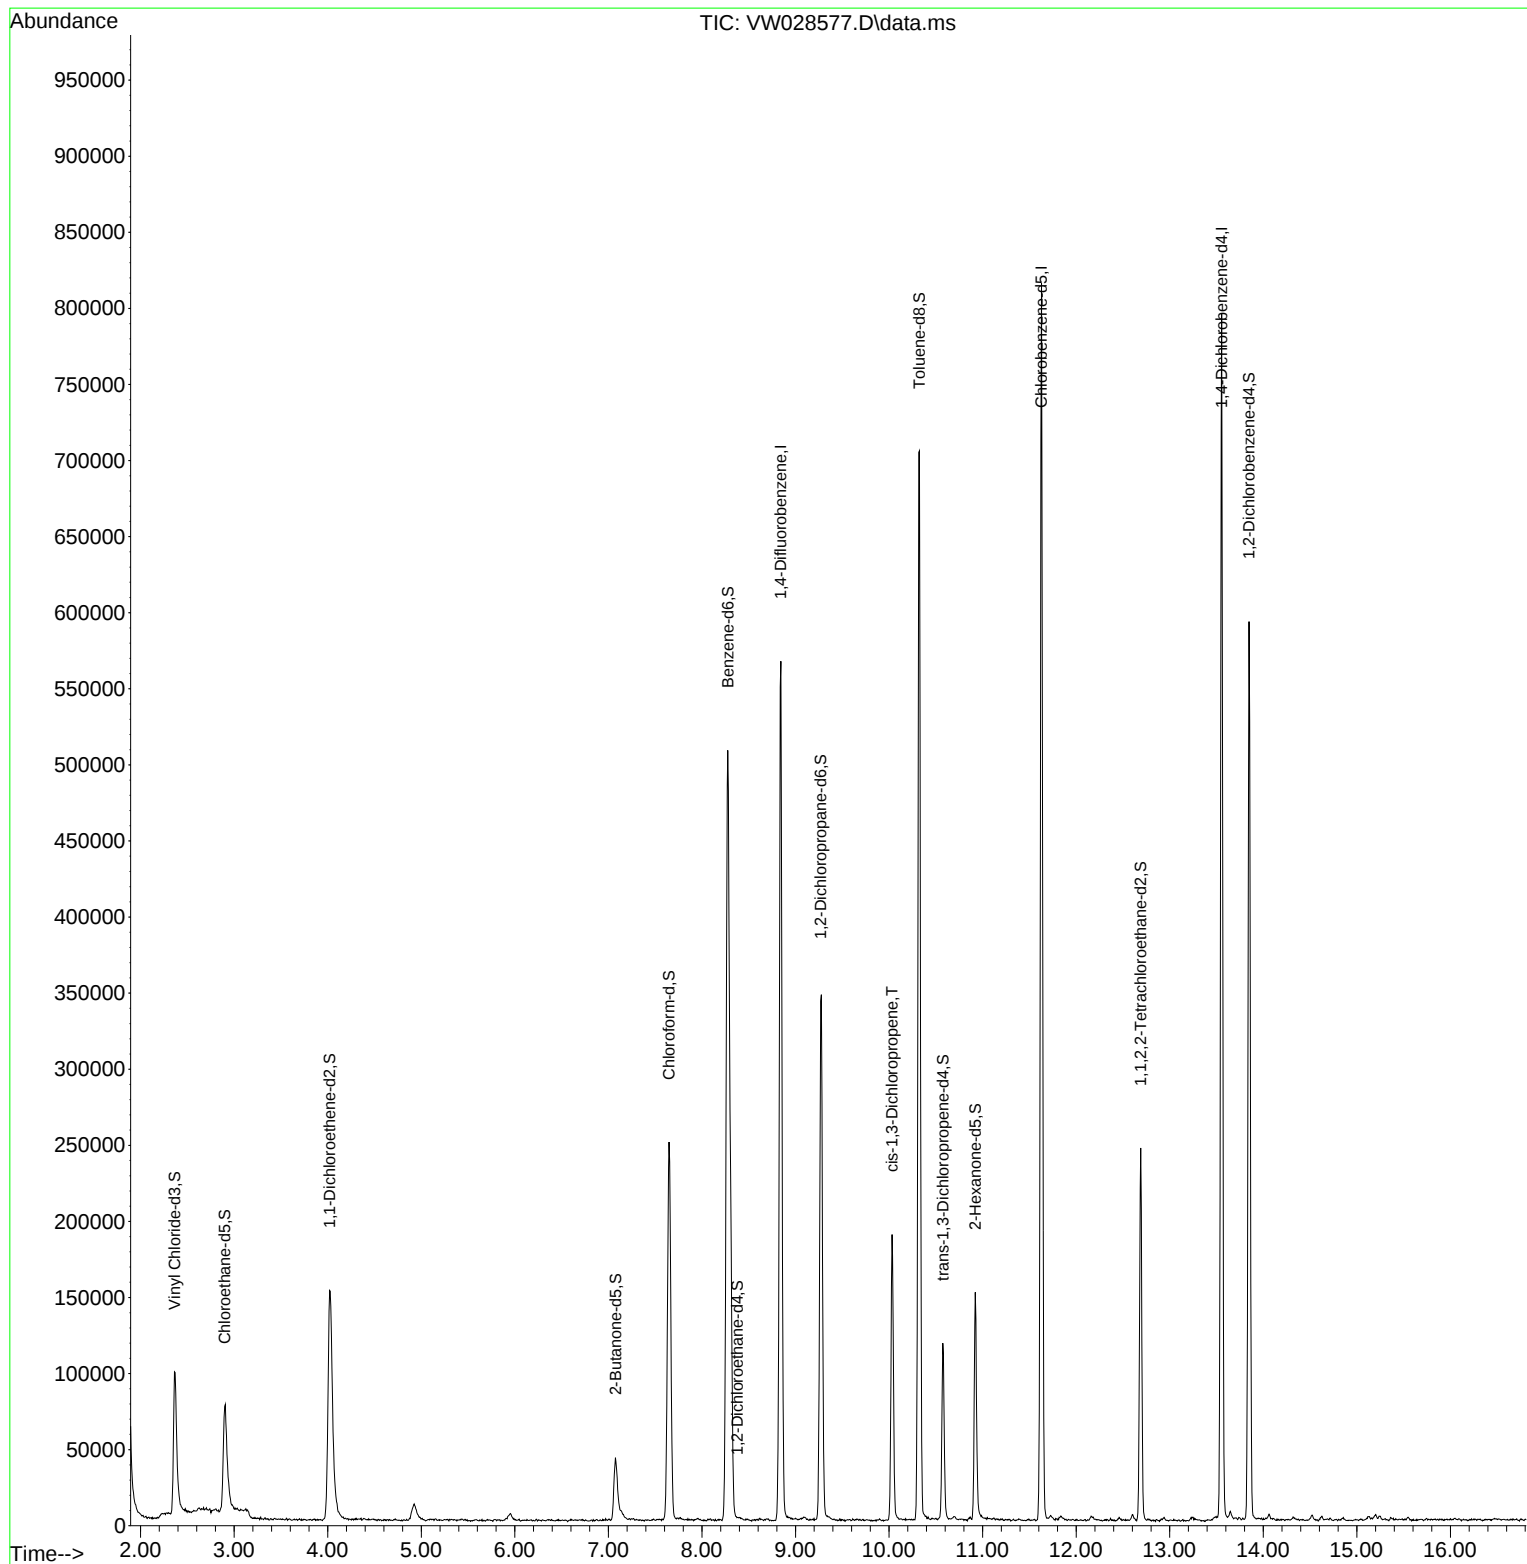

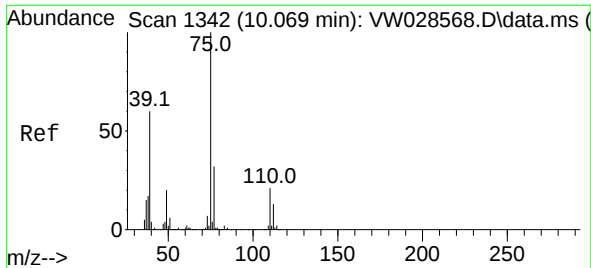

#39
 cis-1,3-Dichloropropene
 Concen: 0.574 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW028577.D
 Acq: 02 May 2024 17:21

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5597
 Ion Ratio Lower Upper
 75 100
 77 33.2 21.8 40.6

