

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022777.D
 Acq On : 03 May 2022 17:14
 Operator : SY/VA
 Sample : N2632-07
 Misc : 5.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 04 01:28:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	269962	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	181065	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	39739	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	152828	27.593	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.360%
7) Chloroethane-d5	2.879	69	108040	29.983	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	119.920%
11) 1,1-Dichloroethene-d2	4.013	63	133982	18.722	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.880%
21) 2-Butanone-d5	7.080	46	63453	60.255	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.500%
24) Chloroform-d	7.653	84	208789	26.398	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.600%
26) 1,2-Dichloroethane-d4	8.403	65	234	0.054	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	394755	37.825	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	151.280%#
36) 1,2-Dichloropropane-d6	9.274	67	116328	39.680	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	158.720%#
41) Toluene-d8	10.323	98	300135	29.770	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	119.080%
43) trans-1,3-Dichloroprop...	10.579	79	39596	29.334	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	117.320%
47) 2-Hexanone-d5	10.927	63	46145	82.454	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	164.900%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85789	31.396	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	125.600%#
66) 1,2-Dichlorobenzene-d4	13.853	152	38359	27.613	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.440%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	3775	0.943	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022777.D
Acq On : 03 May 2022 17:14
Operator : SY/VA
Sample : N2632-07
Misc : 5.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: May 04 01:28:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 01:21:13 2022
Response via : Initial Calibration

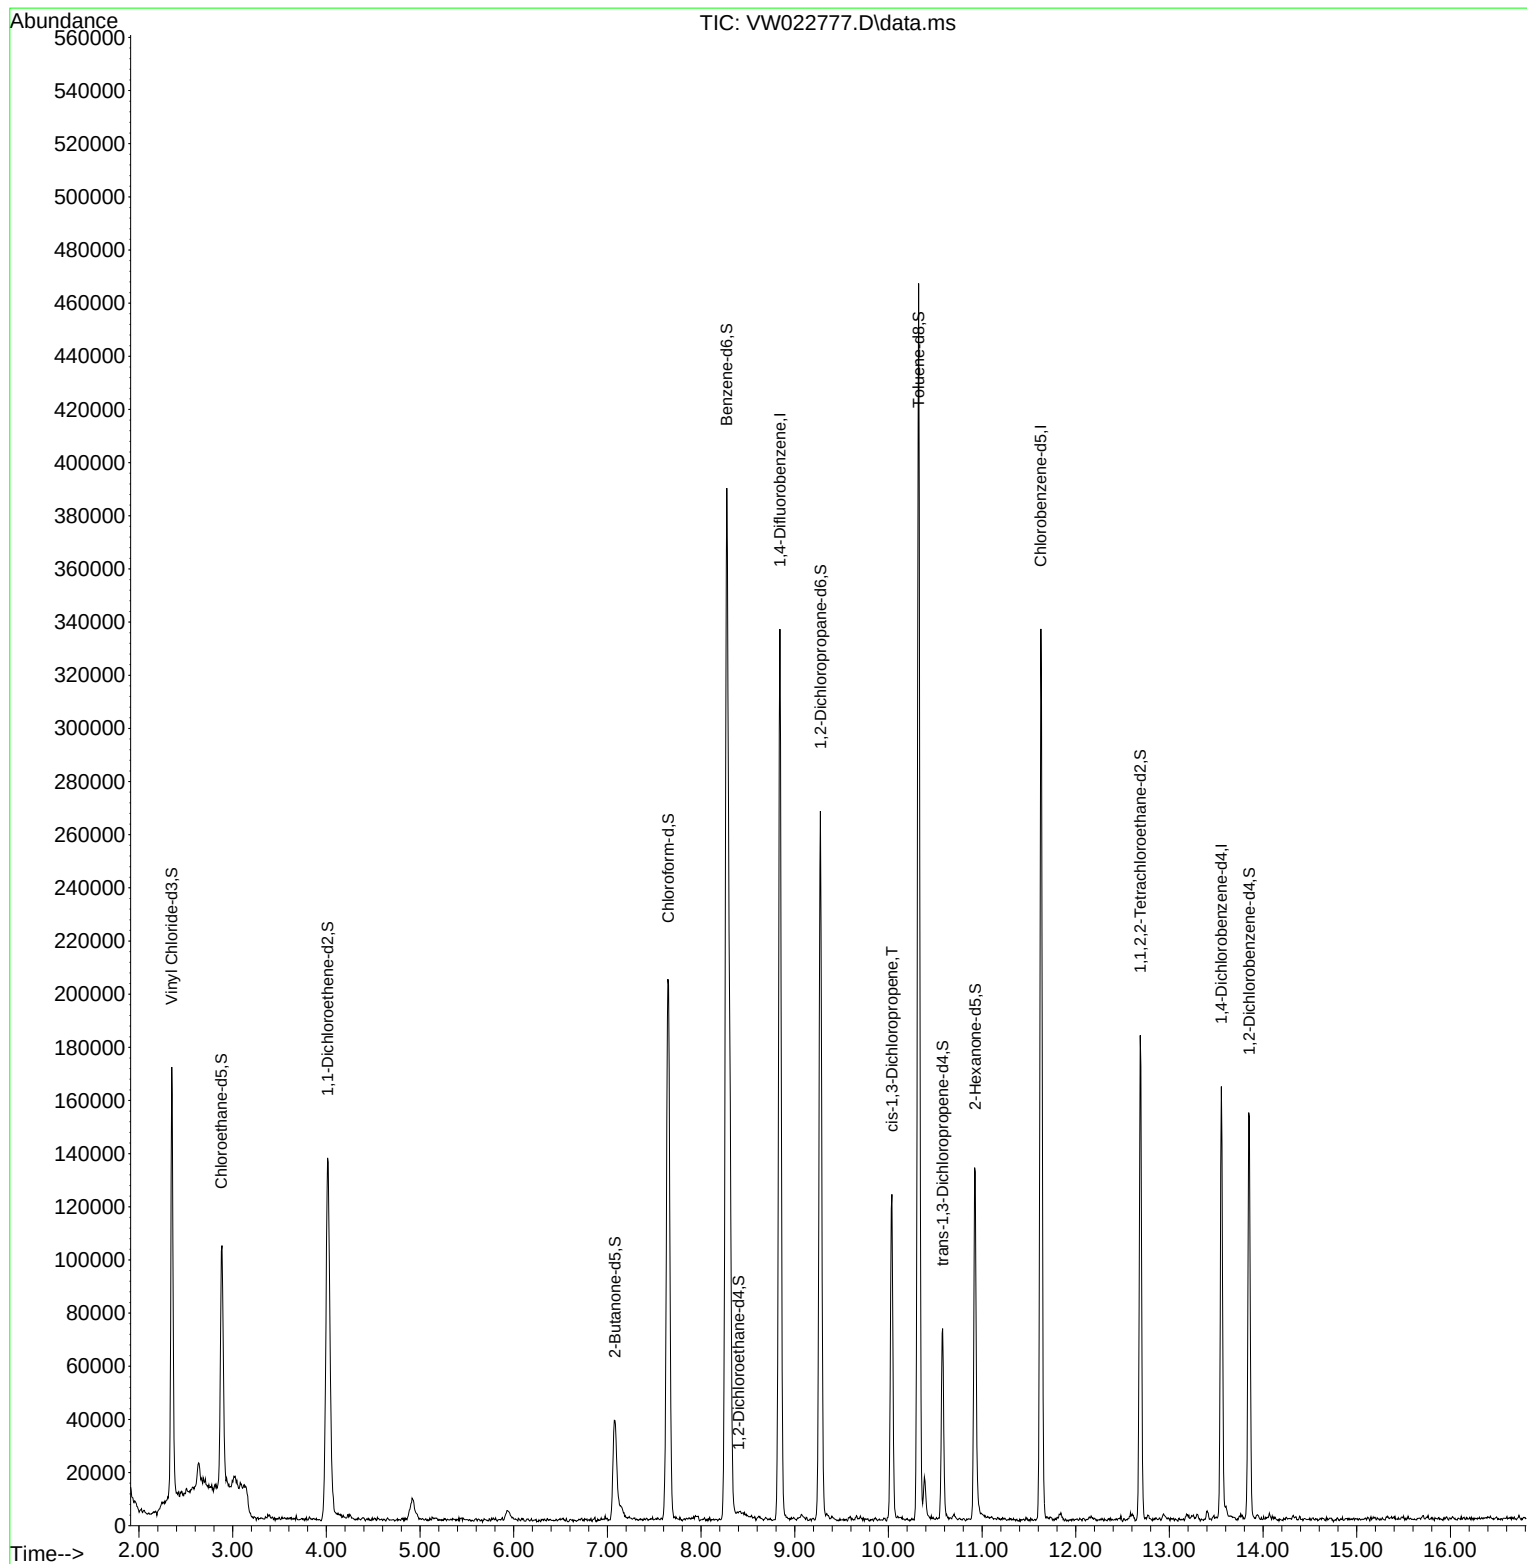

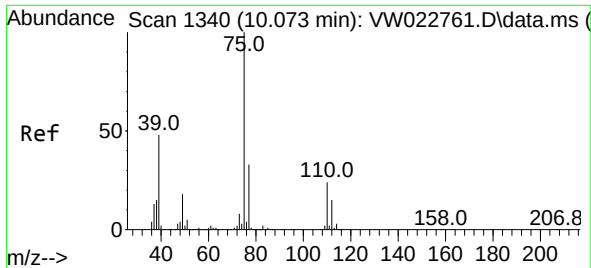

#39
 cis-1,3-Dichloropropene
 Concen: 0.943 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022777.D
 Acq: 03 May 2022 17:14

Instrument :
 MSVOA_W
 ClientSampleId :

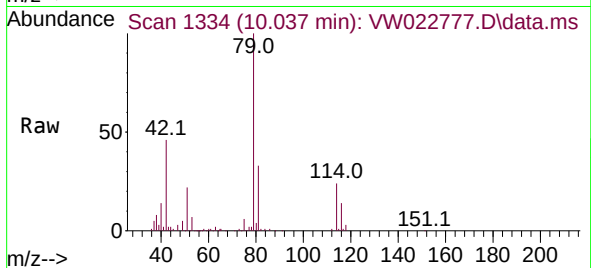

Tgt Ion: 75 Resp: 3775
 Ion Ratio Lower Upper
 75 100
 77 40.1 22.1 41.1

