




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022776.D
Acq On : 03 May 2022 16:50
Operator : SY/VA
Sample : N2632-06
Misc : 7.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4A7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:28:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 01:21:13 2022
Response via : Initial Calibration

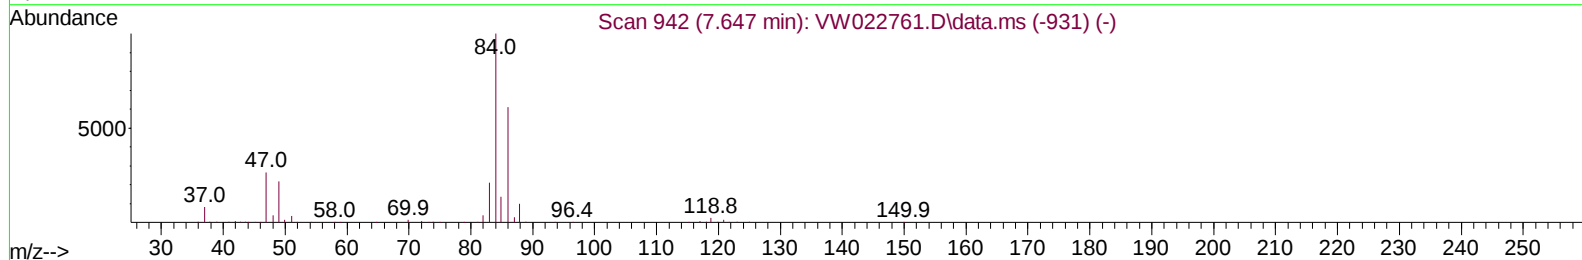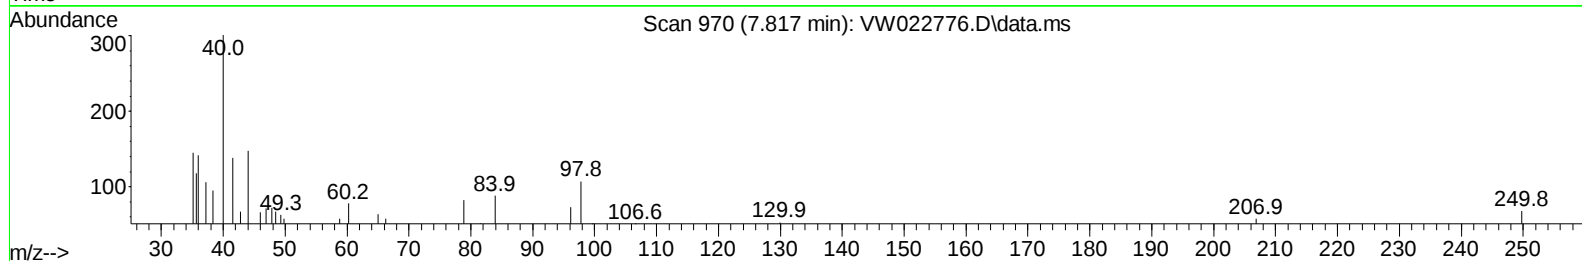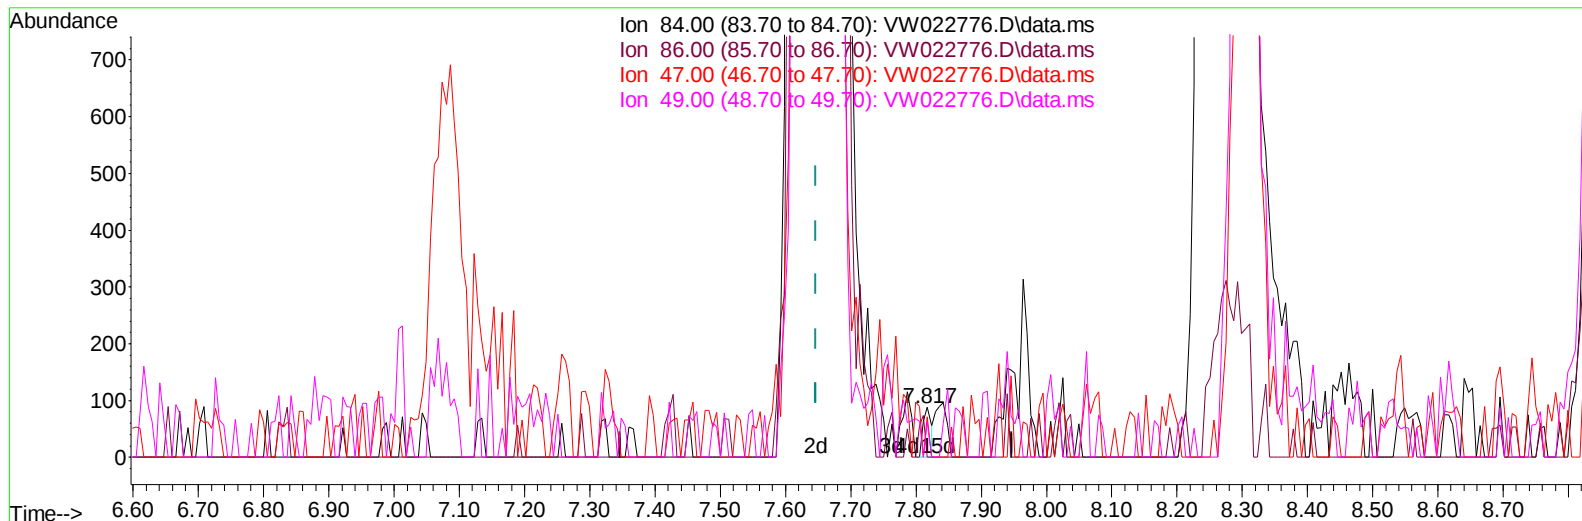

TIC: VW022776.D\data.ms

(24) Chloroform-d (S)

7.817min (+ 0.171) 0.01 ug/L

response 76

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	63.16
47.00	43.20	34.21
49.00	26.40	30.26




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022776.D
Acq On : 03 May 2022 16:50
Operator : SY/VA
Sample : N2632-06
Misc : 7.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4A7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:28:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 01:21:13 2022
Response via : Initial Calibration

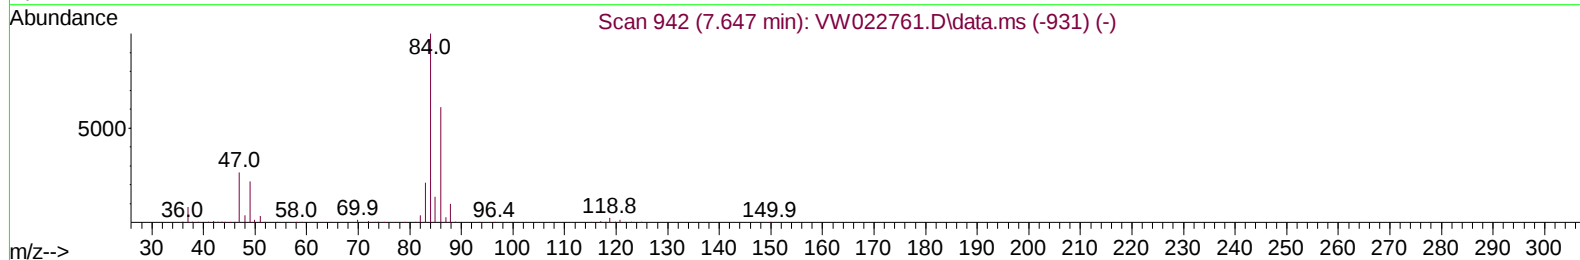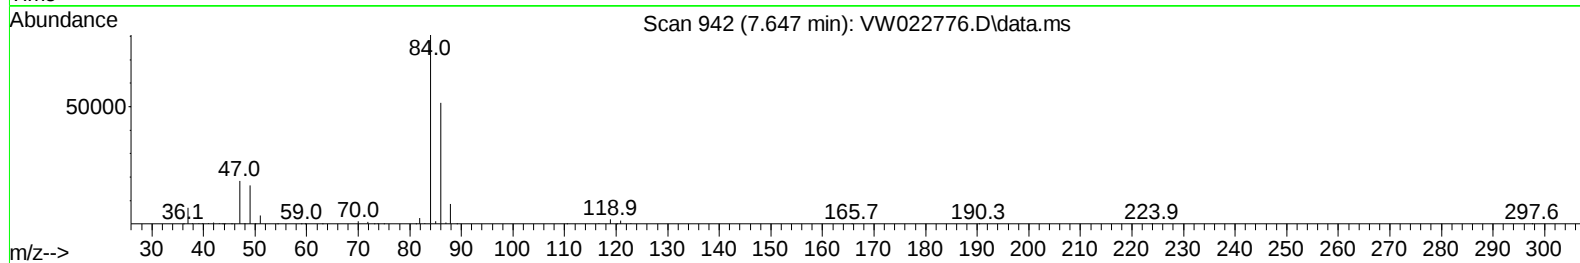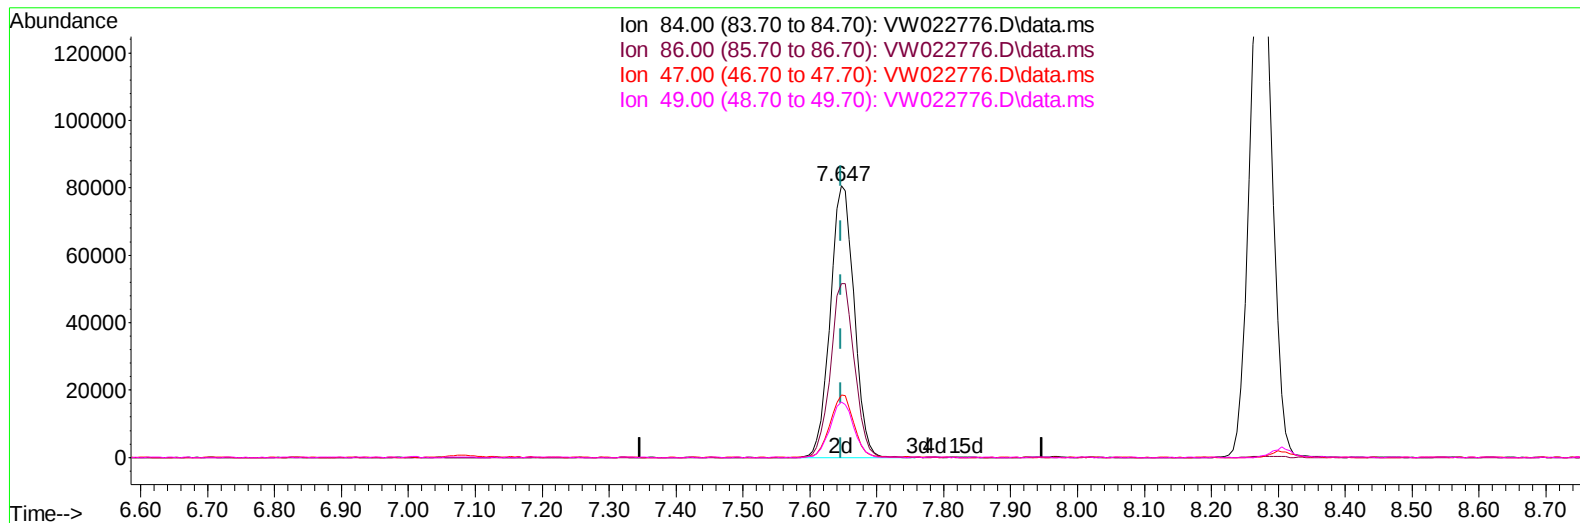

TIC: VW022776.D\data.ms

(24) Chloroform-d (S)

7.647min (+ 0.000) 26.07 ug/L m

response 200064

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	0.02#
47.00	43.20	0.01#
49.00	26.40	0.01#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022776.D
 Acq On : 03 May 2022 16:50
 Operator : SY/VA
 Sample : N2632-06
 Misc : 7.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:28:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	261914	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	195597	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	47646	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	147485	27.446	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	109.800%	
7) Chloroethane-d5	2.885	69	100604	28.778	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	115.120%	
11) 1,1-Dichloroethene-d2	4.013	63	121649	17.521	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	70.080%	
21) 2-Butanone-d5	7.074	46	68734	67.275	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	134.560%	
24) Chloroform-d	7.647	84	200064m	26.072	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	104.280%	
26) 1,2-Dichloroethane-d4	8.305	65	115778	27.510	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	110.040%	
32) Benzene-d6	8.275	84	374391	33.208	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	132.840%	
36) 1,2-Dichloropropane-d6	9.275	67	114605	36.188	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	144.760%#	
41) Toluene-d8	10.323	98	292428	26.851	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	107.400%	
43) trans-1,3-Dichloroprop...	10.579	79	34330	23.543	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	94.160%	
47) 2-Hexanone-d5	10.921	63	46240	76.485	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	152.980%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	98865	33.493	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	133.960%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	53154	31.914	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	127.640%#	
Target Compounds					Qvalue	
13) Acetone	4.129	43	5154	6.738	ug/L	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022776.D
Acq On : 03 May 2022 16:50
Operator : SY/VA
Sample : N2632-06
Misc : 7.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4A7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:28:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 01:21:13 2022
Response via : Initial Calibration

