




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022778.D
 Acq On : 03 May 2022 17:38
 Operator : SY/VA
 Sample : N2632-08
 Misc : 7.11g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:29:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

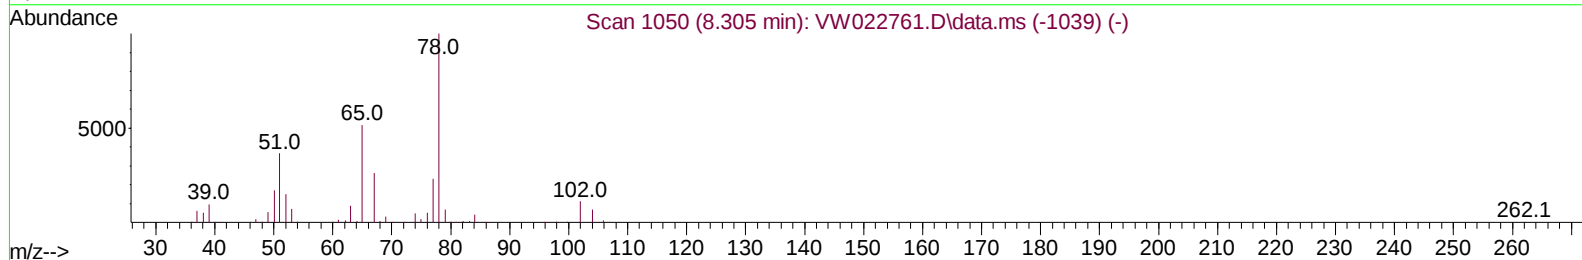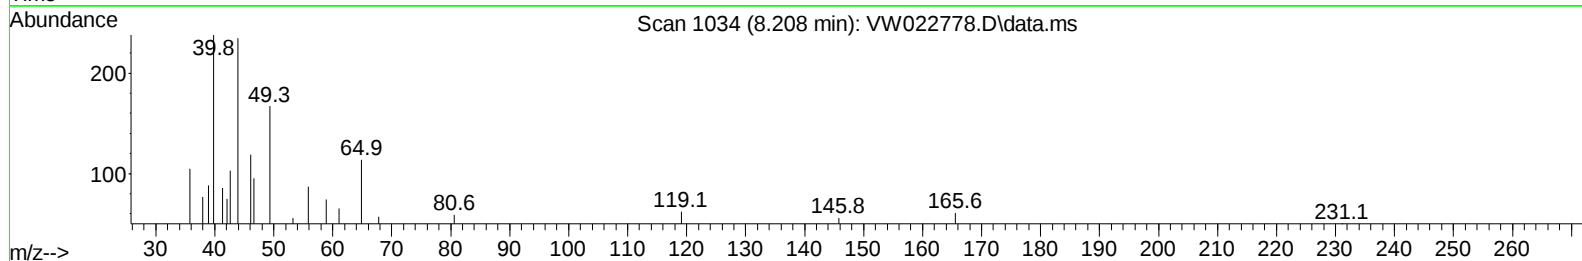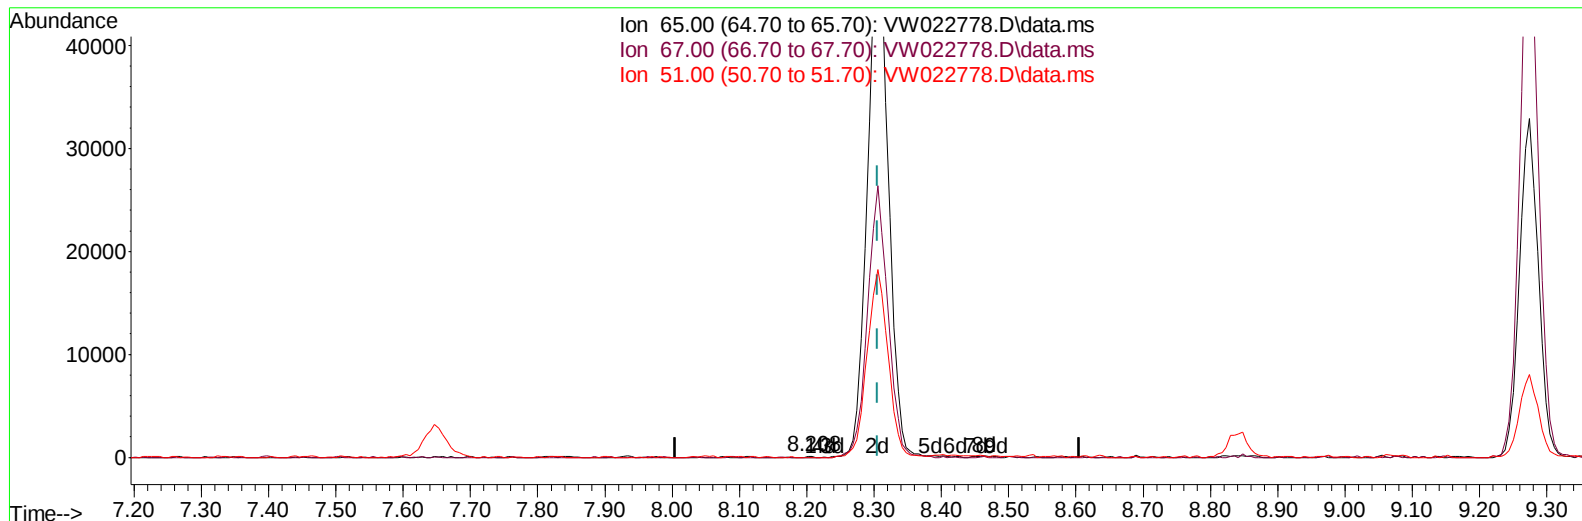

TIC: VW022778.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.208min (-0.097) 0.02 ug/L

response 68

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	63.24
51.00	92.30	113.24
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022778.D
 Acq On : 03 May 2022 17:38
 Operator : SY/VA
 Sample : N2632-08
 Misc : 7.11g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:29:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

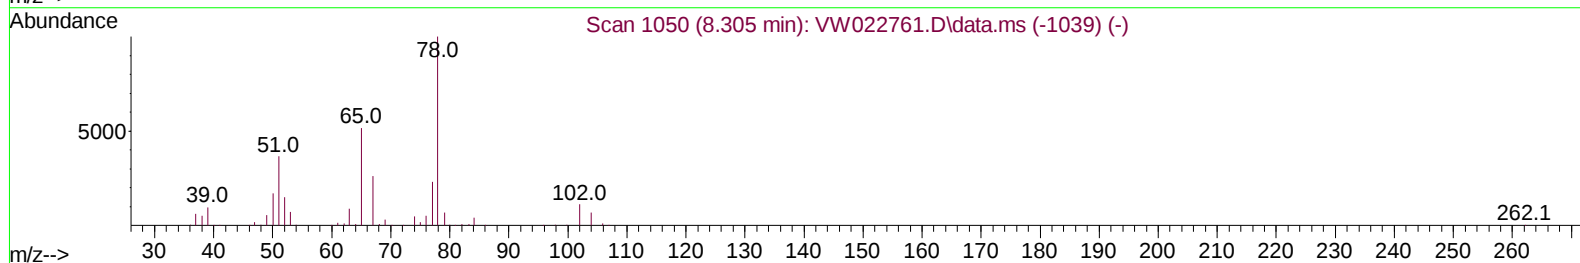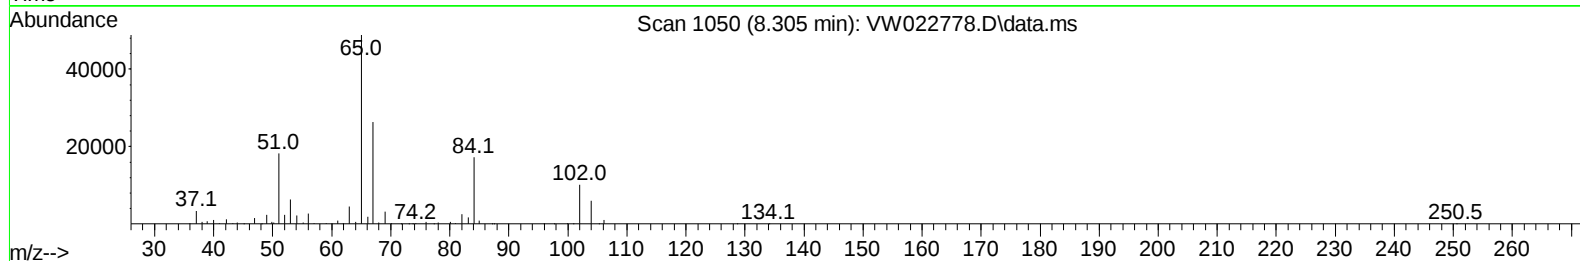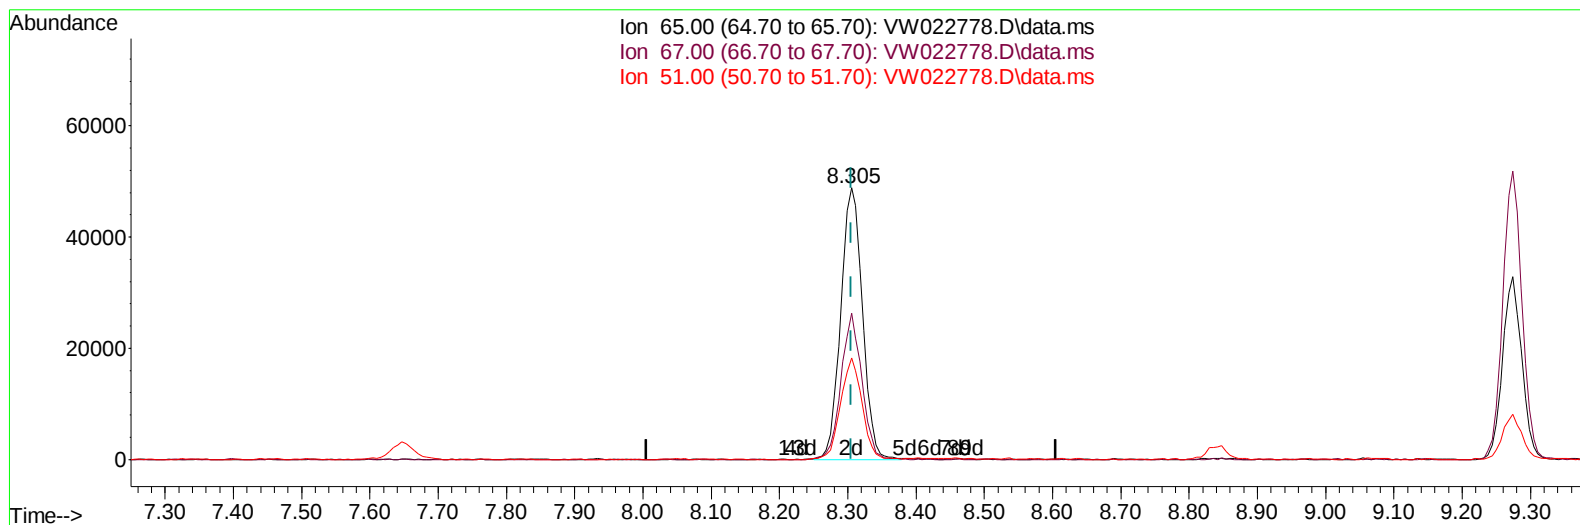

TIC: VW022778.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 27.45 ug/L m

response 107100

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.04#
51.00	92.30	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022778.D
 Acq On : 03 May 2022 17:38
 Operator : SY/VA
 Sample : N2632-08
 Misc : 7.11g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B0

Manual IntegrationsAPPROVED

Quant Time: May 04 01:29:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	242770	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	214305	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	84561	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	122022	24.499	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	98.000%	
7) Chloroethane-d5	2.885	69	85145	26.276	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.120%	
11) 1,1-Dichloroethene-d2	4.019	63	106791	16.593	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.360%	
21) 2-Butanone-d5	7.080	46	57533	60.753	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	121.500%	
24) Chloroform-d	7.647	84	168627	23.708	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	94.840%	
26) 1,2-Dichloroethane-d4	8.305	65	107100m	27.455	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	109.800%	
32) Benzene-d6	8.275	84	332534	26.921	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	107.680%	
36) 1,2-Dichloropropane-d6	9.274	67	101440	29.235	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	116.920%	
41) Toluene-d8	10.323	98	289035	24.223	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	96.880%	
43) trans-1,3-Dichloroprop...	10.579	79	38166	23.889	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.560%	
47) 2-Hexanone-d5	10.921	63	45903	69.300	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	138.600%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	91926	28.424	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	113.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	75685	25.604	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	102.400%	
Target Compounds						
					Qvalue	
13) Acetone	4.135	43	2982	4.206	ug/L	54
25) Chloroform	7.683	83	8707	1.328	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022778.D
Acq On : 03 May 2022 17:38
Operator : SY/VA
Sample : N2632-08
Misc : 7.11g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4B0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:29:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 01:21:13 2022
Response via : Initial Calibration

