




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022779.D
 Acq On : 03 May 2022 18:02
 Operator : SY/VA
 Sample : N2632-09
 Misc : 7.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B1

Manual IntegrationsAPPROVED

Quant Time: May 04 01:29:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

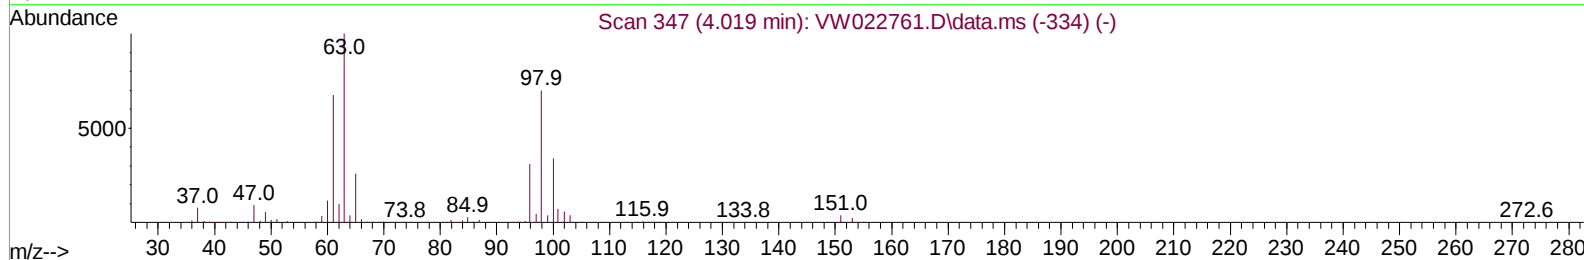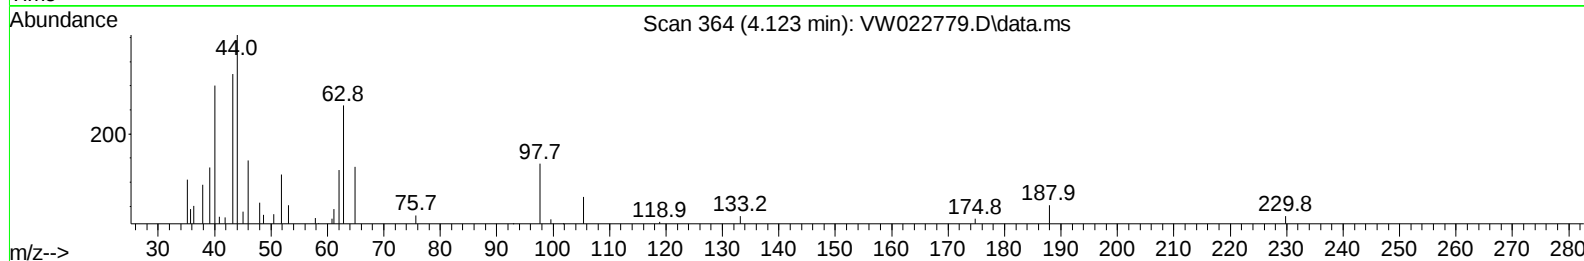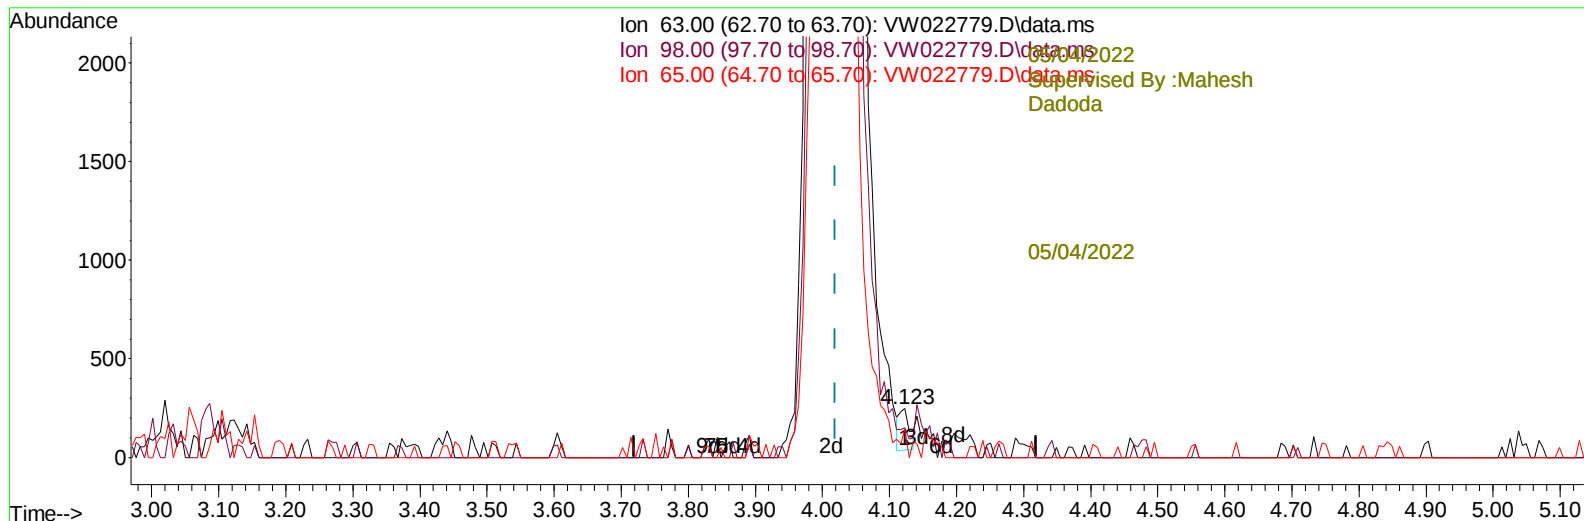

TIC: VW022779.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.123min (+ 0.104) 0.03 ug/L

response 216

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	64.81
65.00	23.30	24.54
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022779.D
 Acq On : 03 May 2022 18:02
 Operator : SY/VA
 Sample : N2632-09
 Misc : 7.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B1

Manual IntegrationsAPPROVED

Quant Time: May 04 01:29:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

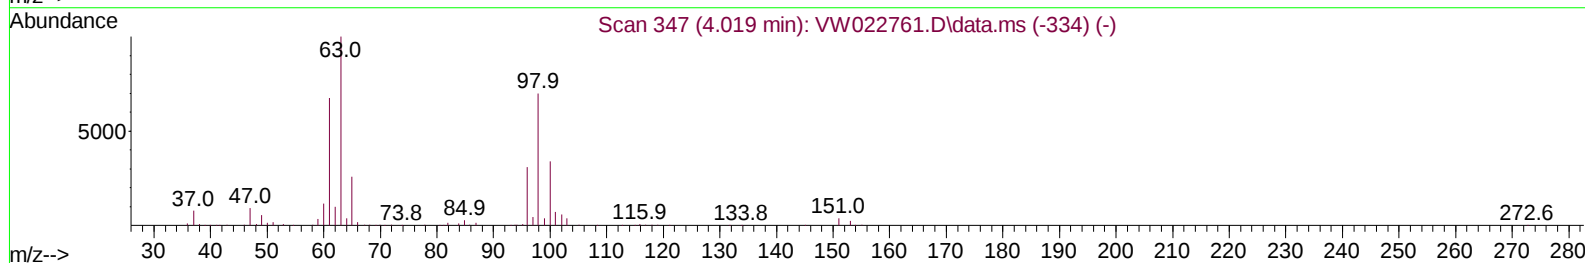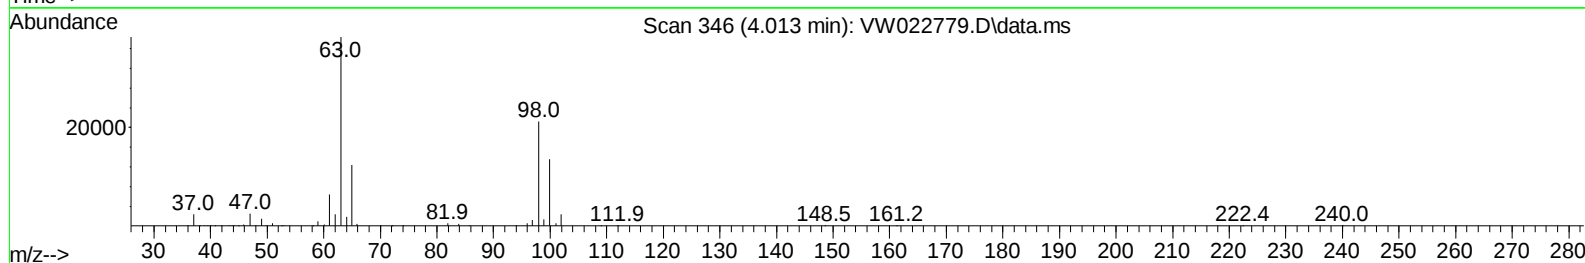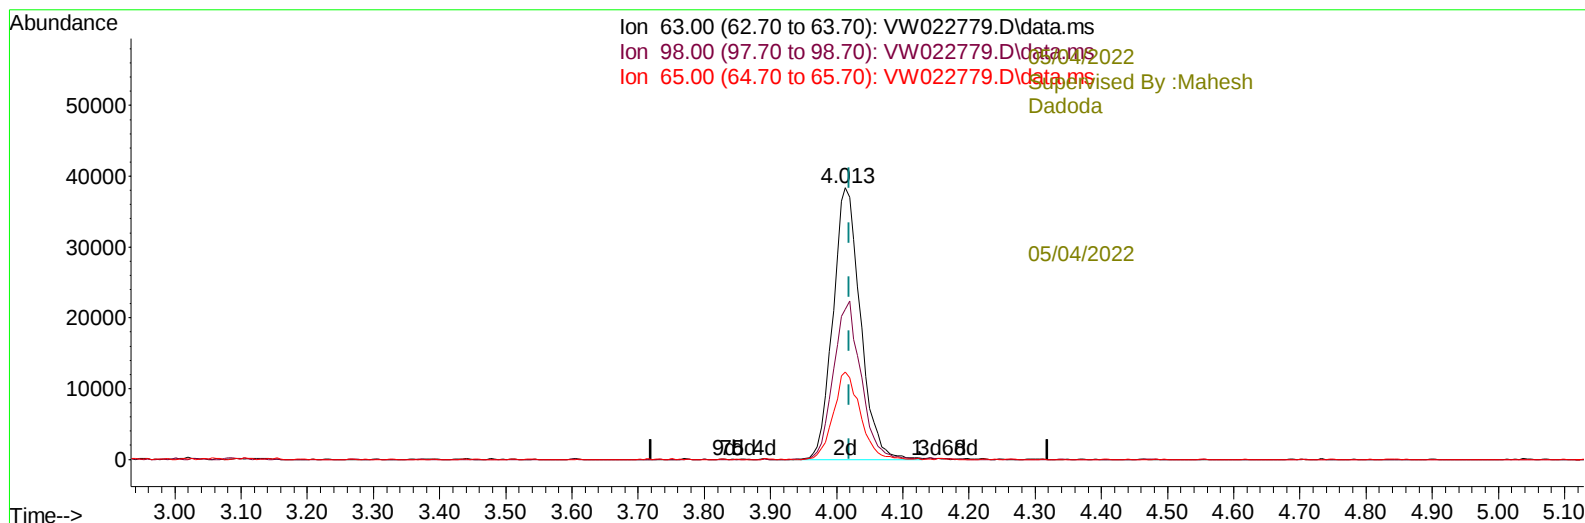

TIC: VW022779.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 16.77 ug/L m

response 110500

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.13#
65.00	23.30	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022779.D
 Acq On : 03 May 2022 18:02
 Operator : SY/VA
 Sample : N2632-09
 Misc : 7.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B1

Manual IntegrationsAPPROVED

Quant Time: May 04 01:29:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 01:21:13 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----05/04/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	248518	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	196581	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	59013	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	129885	25.474	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 101.880%			
7) Chloroethane-d5	2.879	69	89162	26.879	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 107.520%			
11) 1,1-Dichloroethene-d2	4.013	63	110500m	16.773	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 67.080%			
21) 2-Butanone-d5	7.074	46	34606	35.697	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 71.400%			
24) Chloroform-d	7.647	84	182900	25.120	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 100.480%			
26) 1,2-Dichloroethane-d4	8.305	65	108282	27.116	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 108.480%			
32) Benzene-d6	8.275	84	348617	30.767	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 123.080%			
36) 1,2-Dichloropropane-d6	9.275	67	102511	32.207	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 128.840%#			
41) Toluene-d8	10.323	98	291455	26.628	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 106.520%			
43) trans-1,3-Dichloroprop...	10.579	79	36097	24.631	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 98.520%			
47) 2-Hexanone-d5	10.927	63	31494	51.833	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 103.660%			
56) 1,1,2,2-Tetrachloroeth...	12.689	84	89013	30.005	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 120.000%			
66) 1,2-Dichlorobenzene-d4	13.853	152	54754	26.542	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 106.160%			

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022779.D
Acq On : 03 May 2022 18:02
Operator : SY/VA
Sample : N2632-09
Misc : 7.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4B1

Manual IntegrationsAPPROVED

Quant Time: May 04 01:29:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 01:21:13 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

