

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022766.D
 Acq On : 03 May 2022 12:49
 Operator : SY/VA
 Sample : VIBLK443
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK443

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Title : SFAM01.0

Signal : TIC: VW022766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.355	69	74	80	rBV	128333	206935	15.13%	2.272%
2	2.885	157	161	171	rVB	72016	153159	11.20%	1.682%
3	3.202	211	213	216	rBV3	1363	1375	0.10%	0.015%
4	3.672	289	290	294	rBV3	1418	1890	0.14%	0.021%
5	3.727	297	299	301	rVV3	1672	1399	0.10%	0.015%
6	3.763	303	305	307	rVB3	1184	932	0.07%	0.010%
7	3.916	328	330	334	rBV3	856	1050	0.08%	0.012%
8	4.019	336	347	362	rBV	125142	388418	28.40%	4.265%
9	4.208	376	378	383	rVB5	1396	1855	0.14%	0.020%
10	4.251	383	385	388	rBV4	1790	2305	0.17%	0.025%
11	4.330	395	398	400	rBV3	1195	1866	0.14%	0.020%
12	4.391	404	408	420	rVB3	5065	15070	1.10%	0.165%
13	4.617	443	445	446	rVB2	1237	804	0.06%	0.009%
14	4.635	446	448	450	rBV2	735	850	0.06%	0.009%
15	4.684	454	456	457	rBV2	872	674	0.05%	0.007%
16	4.818	475	478	479	rBV3	784	755	0.06%	0.008%
17	4.915	484	494	507	rVB4	9665	39501	2.89%	0.434%
18	5.001	507	508	511	rBV3	979	957	0.07%	0.011%
19	5.062	516	518	520	rBV2	792	830	0.06%	0.009%
20	5.092	521	523	524	rBV	1739	1324	0.10%	0.015%
21	5.312	557	559	561	rVB	1310	1055	0.08%	0.012%
22	5.330	561	562	565	rBV3	1202	886	0.06%	0.010%
23	5.452	580	582	584	rBV3	1282	1025	0.07%	0.011%
24	5.531	593	595	599	rVB4	1273	1309	0.10%	0.014%
25	5.598	603	606	608	rBV2	997	1185	0.09%	0.013%
26	5.665	612	617	619	rVB4	1592	2184	0.16%	0.024%
27	5.702	619	623	624	rBV3	1532	1821	0.13%	0.020%
28	5.897	652	655	656	rBV	917	940	0.07%	0.010%
29	5.933	656	661	662	rBV5	3463	5551	0.41%	0.061%
30	6.092	685	687	690	rBV2	723	798	0.06%	0.009%
31	6.244	709	712	714	rBV4	1236	1389	0.10%	0.015%
32	6.287	718	719	721	rBV2	1053	967	0.07%	0.011%
33	6.372	731	733	737	rVB4	890	1223	0.09%	0.013%
34	6.403	737	738	740	rBV2	1275	705	0.05%	0.008%
35	6.427	740	742	747	rVB5	1141	1362	0.10%	0.015%
36	6.494	750	753	755	rBV3	1248	1654	0.12%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022766.D
 Acq On : 03 May 2022 12:49
 Operator : SY/VA
 Sample : VIBLK443
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK443

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Title : SFAM01.0

37	6.567	762	765	769	rBV5	1164	2059	0.15%	0.023%
38	6.659	778	780	781	rBV2	884	728	0.05%	0.008%
39	6.696	784	786	788	rBV3	1042	839	0.06%	0.009%
40	6.775	796	799	801	rBV2	1445	1724	0.13%	0.019%
41	6.830	804	808	809	rBV3	1170	1180	0.09%	0.013%
42	6.848	809	811	815	rVB4	631	819	0.06%	0.009%
43	6.964	828	830	834	rBV4	796	783	0.06%	0.009%
44	7.006	834	837	838	rBV3	1061	1033	0.08%	0.011%
45	7.080	842	849	854	rBV2	36895	96005	7.02%	1.054%
46	7.409	902	903	904	rBV	1276	671	0.05%	0.007%
47	7.537	920	924	926	rBV4	1138	1357	0.10%	0.015%
48	7.555	926	927	931	rVV4	1136	979	0.07%	0.011%
49	7.653	931	943	954	rVV	202063	497158	36.35%	5.459%
50	7.842	972	974	976	rBV3	696	663	0.05%	0.007%
51	7.878	976	980	981	rBV3	1448	1245	0.09%	0.014%
52	8.079	1011	1013	1014	rBV2	1098	801	0.06%	0.009%
53	8.275	1033	1045	1060	rBV3	438549	1367633	100.00%	15.017%
54	8.738	1119	1121	1124	rVB2	1067	729	0.05%	0.008%
55	8.841	1129	1138	1150	rVV	359822	706749	51.68%	7.760%
56	8.988	1160	1162	1163	rVB	1305	686	0.05%	0.008%
57	9.030	1166	1169	1172	rBV4	1566	2035	0.15%	0.022%
58	9.274	1201	1209	1222	rBV	266050	534257	39.06%	5.866%
59	9.713	1279	1281	1283	rBV2	1719	1222	0.09%	0.013%
60	9.762	1283	1289	1294	rVV7	3349	7262	0.53%	0.080%
61	9.890	1300	1310	1317	rBV4	9604	21377	1.56%	0.235%
62	9.939	1317	1318	1321	rBV2	949	1088	0.08%	0.012%
63	9.969	1321	1323	1324	rBV2	2286	1595	0.12%	0.018%
64	10.036	1327	1334	1341	rVV	138126	248029	18.14%	2.723%
65	10.323	1373	1381	1388	rBV	569407	995217	72.77%	10.928%
66	10.579	1416	1423	1430	rBV	88757	154895	11.33%	1.701%
67	10.701	1435	1443	1451	rBV	24489	45936	3.36%	0.504%
68	10.926	1473	1480	1492	rBV	145473	263586	19.27%	2.894%
69	11.067	1497	1503	1508	rVV4	9994	17224	1.26%	0.189%
70	11.170	1516	1520	1528	rVB5	3781	7220	0.53%	0.079%
71	11.231	1528	1530	1535	rBV5	1009	1602	0.12%	0.018%
72	11.432	1555	1563	1569	rVB3	10431	21522	1.57%	0.236%
73	11.628	1586	1595	1604	rBV	540397	908283	66.41%	9.973%
74	11.823	1623	1627	1632	rBV7	2403	5013	0.37%	0.055%
75	11.896	1637	1639	1642	rVB4	1050	1019	0.07%	0.011%
76	11.945	1644	1647	1649	rBV3	1006	914	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
 Data File : VW022766.D
 Acq On : 03 May 2022 12:49
 Operator : SY/VA
 Sample : VIBLK443
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK443

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Title : SFAM01.0

77	12.140	1678	1679	1681	rBV2	1274	1119	0.08%	0.012%
78	12.341	1709	1712	1713	rBV2	1028	887	0.06%	0.010%
79	12.457	1729	1731	1732	rBV2	1634	1126	0.08%	0.012%
80	12.603	1748	1755	1762	rVB3	21488	40613	2.97%	0.446%
81	12.688	1762	1769	1776	rBV	236231	396740	29.01%	4.356%
82	12.743	1776	1778	1780	rBV3	2096	1754	0.13%	0.019%
83	12.847	1792	1795	1796	rBV3	1159	1462	0.11%	0.016%
84	12.883	1799	1801	1802	rVV2	1143	708	0.05%	0.008%
85	12.938	1806	1810	1818	rVB10	4097	9522	0.70%	0.105%
86	13.005	1820	1821	1825	rBV4	1792	2343	0.17%	0.026%
87	13.188	1848	1851	1856	rVB4	4599	7097	0.52%	0.078%
88	13.237	1857	1859	1864	rBV4	2319	3637	0.27%	0.040%
89	13.469	1894	1897	1898	rBV2	2884	2547	0.19%	0.028%
90	13.554	1904	1911	1924	rBV	565710	960612	70.24%	10.548%
91	13.853	1953	1960	1970	rVB	507692	861049	62.96%	9.455%
92	14.066	1991	1995	2002	rVB2	9338	15638	1.14%	0.172%
93	14.316	2033	2036	2037	rBV2	1603	1809	0.13%	0.020%
94	14.377	2044	2046	2049	rVB4	2196	1554	0.11%	0.017%
95	14.718	2099	2102	2108	rVB8	4251	6307	0.46%	0.069%
96	14.987	2145	2146	2147	rBV	1143	765	0.06%	0.008%
97	15.432	2214	2219	2224	rBV3	10481	16983	1.24%	0.186%
98	15.919	2297	2299	2301	rBV3	1305	1377	0.10%	0.015%
99	15.974	2306	2308	2310	rBV3	1166	1433	0.10%	0.016%
100	16.743	2432	2434	2436	rBV2	1141	852	0.06%	0.009%




Sum of corrected areas: 9107074

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022766.D
Acq On : 03 May 2022 12:49
Operator : SY/VA
Sample : VIBLK443
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK443

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

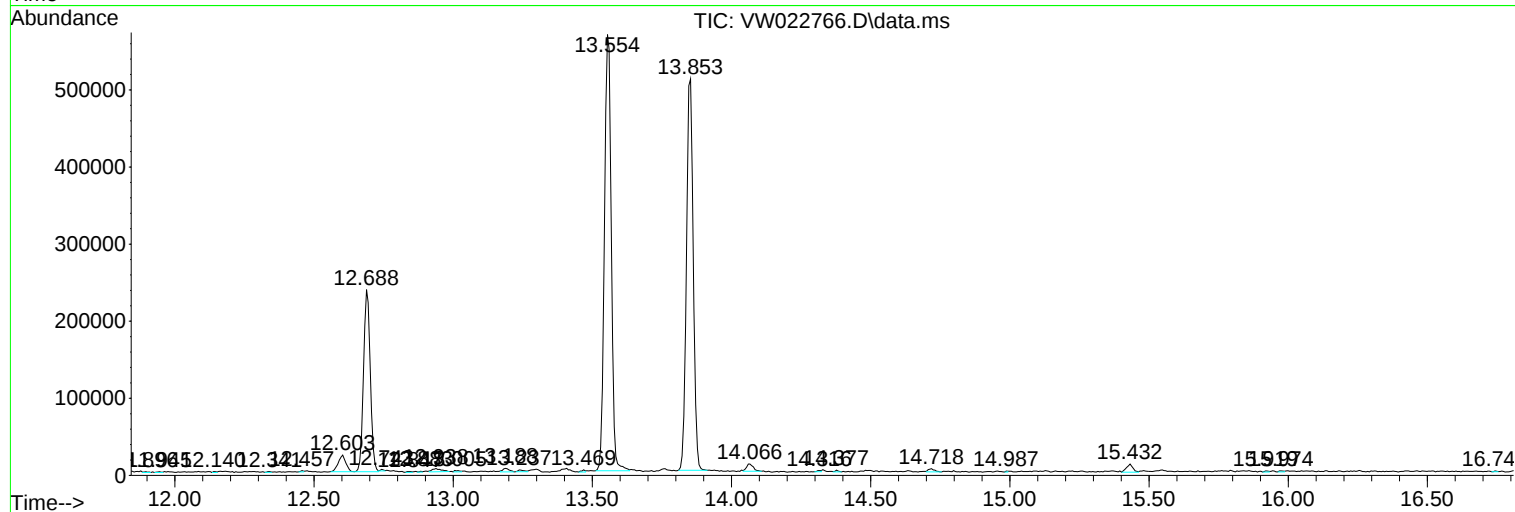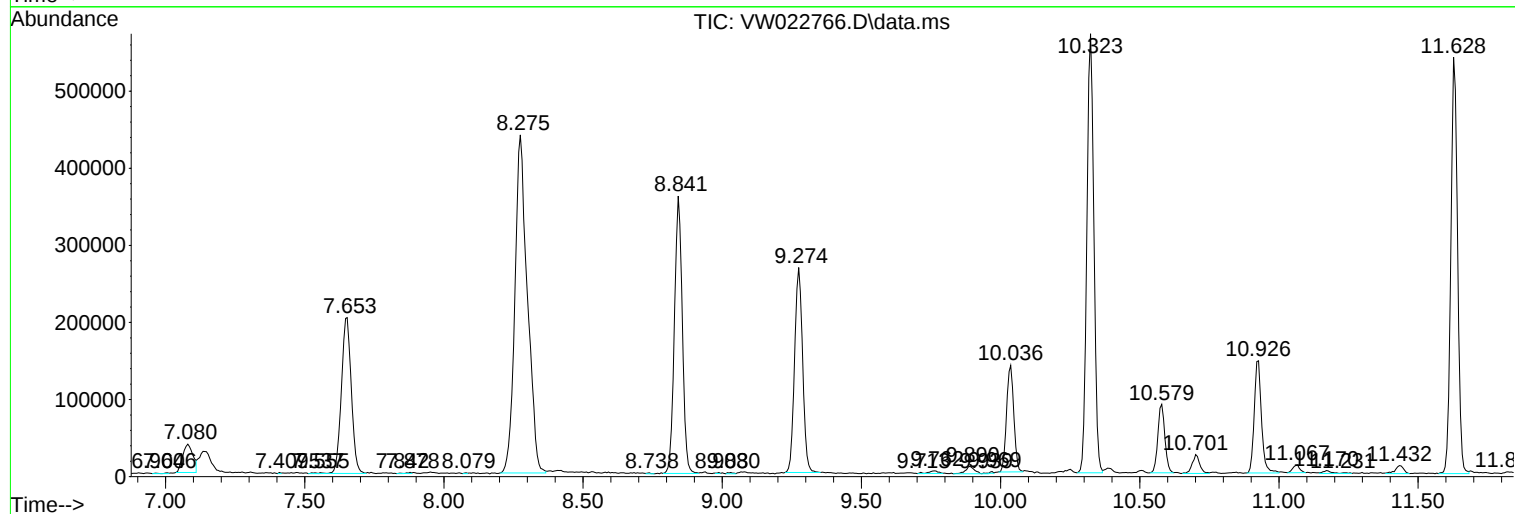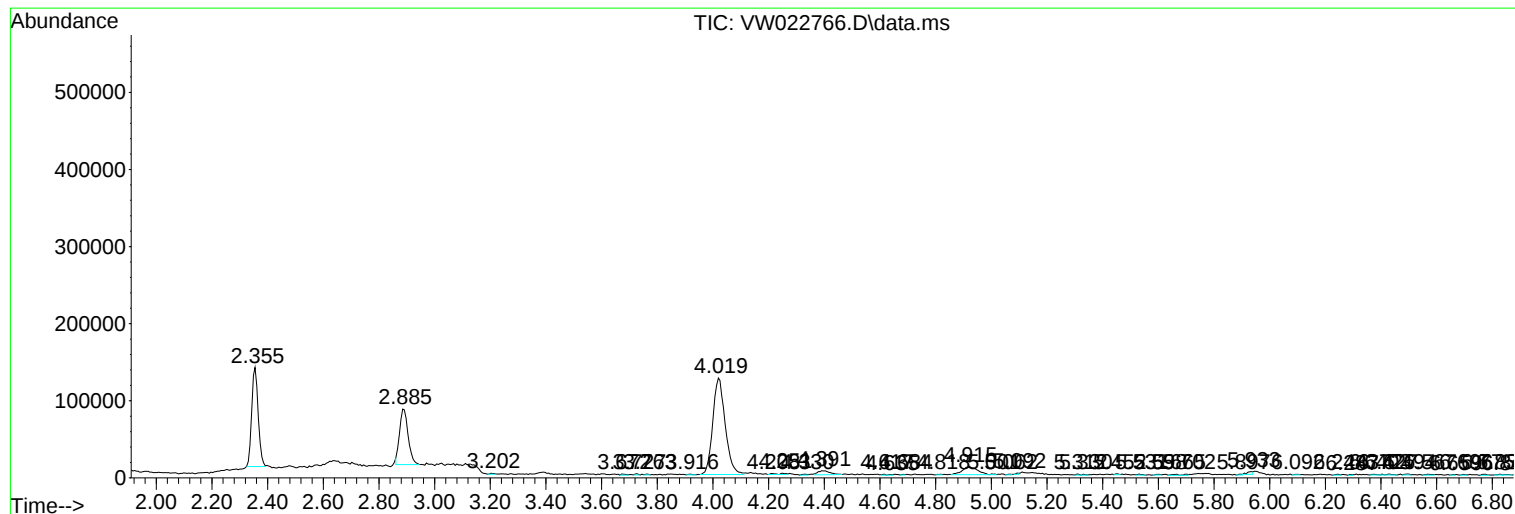

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022766.D
Acq On : 03 May 2022 12:49
Operator : SY/VA
Sample : VIBLK443
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK443

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022766.D
Acq On : 03 May 2022 12:49
Operator : SY/VA
Sample : VIBLK443
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK443

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc