


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050322\
Data File : VW022760.D
Acq On : 03 May 2022 09:33
Operator : SY/VA
Sample : BFB546
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB546

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Title : SFAM01.0
Last Update : Sat May 07 01:54:32 2022

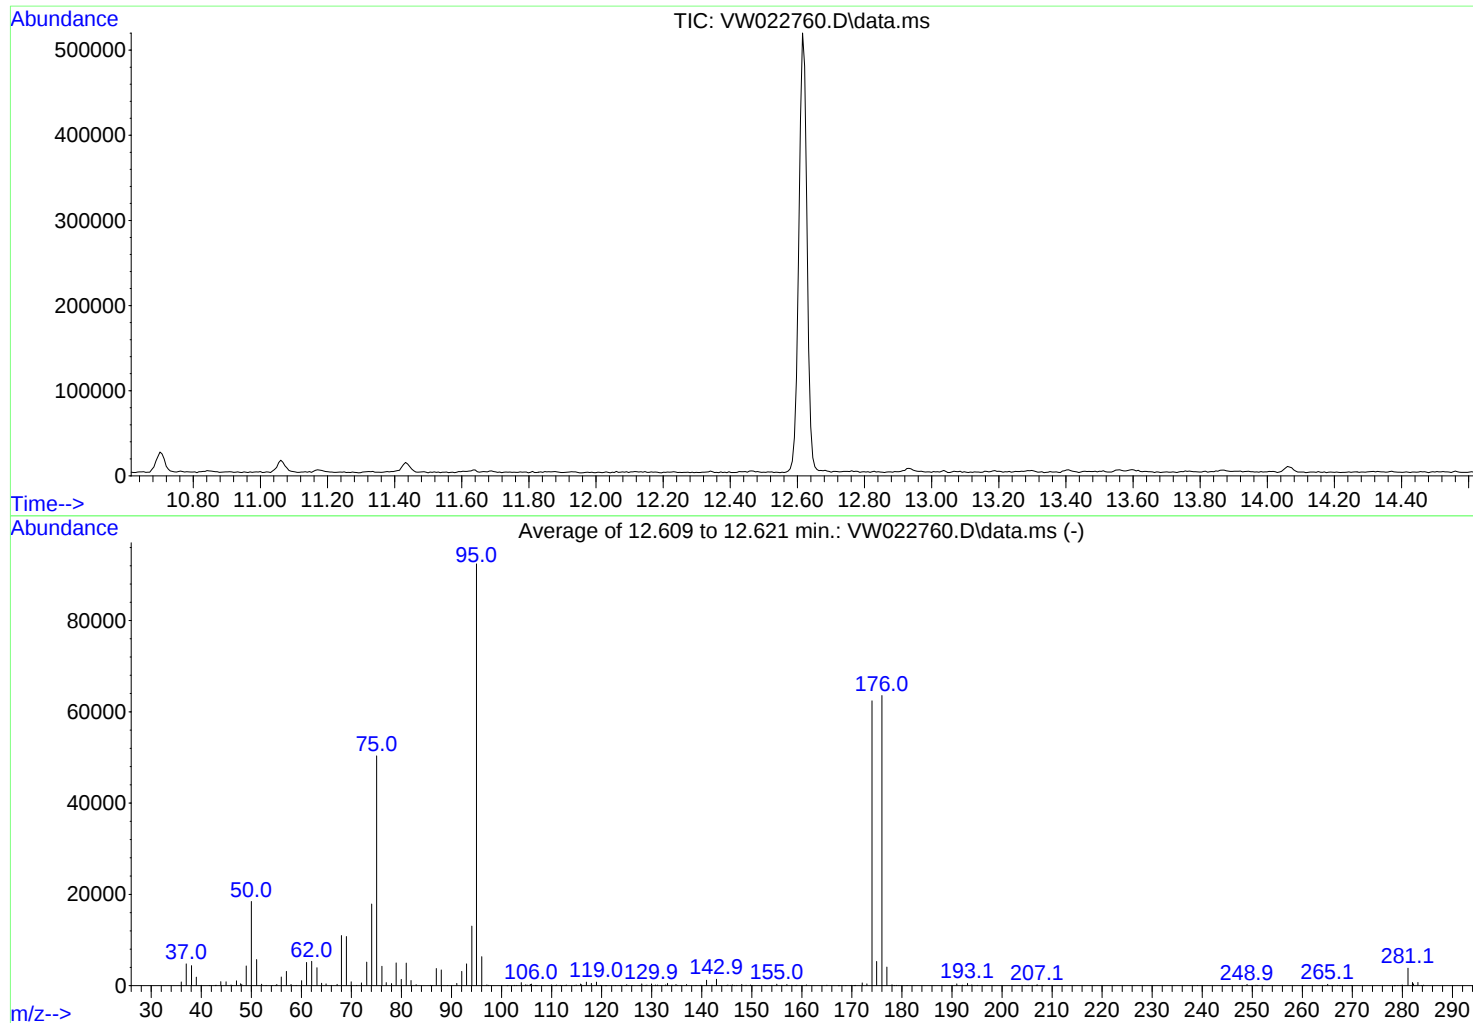

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	18440	PASS
75	95	30	80	54.5	50340	PASS
95	95	100	100	100.0	92419	PASS
96	95	5	9	6.9	6348	PASS
173	174	0.00	2	0.6	399	PASS
174	95	50	120	67.5	62408	PASS
175	174	5	9	8.5	5283	PASS
176	174	95	105	101.8	63552	PASS
177	176	5	10	6.4	4078	PASS

m/z	Abundance
35.40	135.0
36.00	58.0
36.50	92.0
37.00	91.0
38.20	76.0
39.10	111.0
40.00	2455.0
41.00	166.0
43.90	210.0
44.90	55.0
46.60	52.0
51.70	55.0
53.40	66.0
54.90	63.0
56.10	95.0
57.20	120.0
59.00	63.0
66.60	111.0
68.50	70.0
72.30	107.0
75.30	95.0
81.90	70.0
86.30	57.0
87.00	50.0
93.00	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB546

m/z	Abundance
36.00	695.0
37.00	4323.0
38.00	4224.0
39.00	1851.0
40.00	2770.0
41.10	127.0
42.80	152.0
44.00	1115.0
45.00	883.0
46.20	138.0
47.10	751.0
47.90	735.0
49.00	4176.0
50.00	16920.0
51.00	5183.0
52.10	201.0
52.90	54.0
54.90	378.0
56.00	1959.0
57.00	2684.0
58.00	155.0
58.90	219.0
60.00	757.0
61.10	4494.0
62.10	5464.0
63.10	3761.0
64.10	537.0
65.00	479.0
66.60	57.0
67.20	172.0
68.00	10069.0
69.00	9139.0
70.00	679.0
71.00	101.0
72.10	659.0
73.10	5339.0
74.00	16640.0
75.10	45544.0
76.10	4019.0
77.00	704.0
78.00	446.0
78.90	4455.0
79.90	1428.0
81.00	4364.0
82.00	1064.0
82.90	279.0
85.80	57.0
86.20	73.0
86.90	3368.0
88.00	3227.0
89.20	139.0
91.00	557.0
92.00	2766.0
93.00	4144.0
94.00	11155.0
95.00	81832.0
96.00	5696.0
97.40	218.0
101.10	51.0
103.00	167.0
104.00	400.0
104.90	311.0
105.70	494.0
106.00	395.0
106.70	75.0
107.10	64.0
110.00	157.0
110.80	130.0
111.80	62.0
113.00	231.0
115.00	144.0
115.80	582.0
116.90	758.0
118.00	465.0
119.00	697.0
119.80	139.0
120.80	56.0
125.00	320.0
126.20	56.0
127.70	239.0
128.10	292.0
129.00	216.0
130.00	370.0
130.80	208.0
133.20	689.0
134.00	99.0
134.90	268.0
137.00	254.0
139.80	109.0
141.00	993.0
143.00	1141.0
144.90	196.0

Instrument :
MSVOA_W
ClientSampleId :
BFB546

145.80	236.0
146.50	145.0
148.10	243.0
148.90	221.0
149.80	223.0
153.00	96.0
153.80	77.0
155.00	313.0
157.00	165.0
158.10	94.0
158.70	129.0
161.00	156.0
164.90	155.0
169.80	53.0
172.10	614.0
173.00	1196.0
174.00	49680.0
174.90	4763.0
176.00	48648.0
177.10	3447.0
178.00	113.0
178.90	241.0
179.40	155.0
181.00	64.0
190.90	421.0
192.10	217.0
193.10	760.0
193.90	180.0
195.10	85.0
205.20	87.0
206.90	336.0
208.10	151.0
239.00	57.0
248.90	506.0
249.80	85.0
250.70	206.0
251.10	183.0
252.20	102.0
265.10	585.0
265.90	129.0
267.00	157.0
267.50	57.0
269.80	60.0
278.40	56.0
279.10	77.0
280.00	239.0
281.10	5184.0
282.00	1469.0
283.10	907.0
283.80	154.0
284.20	147.0

Instrument :
MSVOA_W
ClientSampleId :
BFB546

m/z	Abundance
36.00	1008.0
37.00	5785.0
38.00	5076.0
39.00	2277.0
40.00	2506.0
41.10	138.0
43.00	166.0
44.00	1185.0
45.00	1009.0
45.90	167.0
47.00	1330.0
48.10	723.0
49.00	4834.0
50.00	21008.0
51.10	6172.0
52.00	404.0
53.00	112.0
54.20	51.0
55.10	463.0
56.00	2241.0
57.00	3524.0
57.90	374.0
59.00	76.0
60.00	1353.0
61.00	5901.0
62.00	5663.0
63.10	4320.0
64.00	602.0
64.90	383.0
66.00	156.0
67.20	392.0
68.00	12843.0
69.00	12269.0
69.90	1028.0
71.90	687.0
73.00	5292.0
74.10	20592.0
75.10	57232.0
76.10	4341.0
77.00	803.0
78.10	445.0
79.00	5872.0
80.00	1669.0
80.90	5257.0
81.90	1325.0
83.00	176.0
85.80	213.0
87.00	4263.0
88.00	3757.0
91.00	513.0
92.00	3653.0
93.00	5131.0
94.10	14221.0
95.00	103064.0
96.10	7187.0
97.10	246.0
102.60	91.0
103.90	924.0
104.70	213.0
105.20	217.0
105.90	699.0
106.80	118.0
109.80	134.0
111.00	274.0
111.80	157.0
112.70	205.0
114.60	146.0
115.00	129.0
116.00	530.0
117.00	742.0
117.90	539.0
118.90	703.0
119.80	56.0
123.80	147.0
125.00	348.0
127.90	443.0
129.10	242.0
130.00	427.0
130.70	179.0
131.20	200.0
131.80	85.0
132.80	481.0
133.20	622.0
134.10	201.0
134.90	358.0
135.90	94.0
137.00	268.0
138.80	104.0
139.90	55.0
141.00	1412.0
142.10	273.0
142.90	1622.0

Instrument :
MSVOA_W
ClientSampleId :
BFB546

143.90	63.0
145.20	185.0
146.20	220.0
147.00	128.0
148.10	158.0
148.80	90.0
149.70	161.0
152.70	108.0
153.90	66.0
154.90	443.0
156.00	60.0
157.00	263.0
158.00	65.0
159.00	126.0
160.90	207.0
165.00	88.0
169.90	140.0
170.50	145.0
172.00	699.0
174.00	64040.0
175.00	5653.0
176.00	68048.0
176.90	4617.0
178.00	161.0
178.50	69.0
191.00	432.0
192.10	82.0
193.10	502.0
194.00	150.0
195.00	188.0
204.80	99.0
205.20	81.0
207.10	317.0
207.80	66.0
239.10	105.0
249.00	231.0
250.80	148.0
252.10	89.0
264.90	164.0
266.10	80.0
269.80	58.0
279.90	220.0
281.10	4161.0
282.20	1176.0
283.10	722.0
284.30	131.0

Instrument :
MSVOA_W
ClientSampleId :
BFB546

m/z	Abundance
36.00	937.0
37.00	4479.0
38.10	4037.0
39.00	1776.0
40.00	2325.0
40.90	78.0
41.70	73.0
42.90	139.0
43.90	986.0
45.00	836.0
46.00	262.0
47.10	1091.0
47.80	565.0
49.00	3889.0
50.00	17392.0
51.00	5777.0
52.10	303.0
52.90	60.0
53.50	74.0
54.10	94.0
55.10	273.0
56.00	1779.0
57.00	3553.0
58.00	219.0
59.00	89.0
60.10	1202.0
61.00	4883.0
62.00	4820.0
63.10	3671.0
64.10	478.0
64.90	265.0
66.00	61.0
67.10	260.0
68.00	10028.0
69.00	10880.0
69.90	882.0
71.00	167.0
72.10	399.0
73.00	4880.0
74.10	16384.0
75.00	48528.0
76.10	4350.0
76.90	518.0
77.90	532.0
78.90	4610.0
80.00	1027.0
80.90	5230.0
82.00	1187.0
83.00	217.0
86.10	249.0
87.00	3780.0
87.90	3349.0
91.10	452.0
92.10	2999.0
93.00	5148.0
94.00	13801.0
95.00	92360.0
96.10	6160.0
97.00	244.0
102.60	85.0
103.00	69.0
104.00	728.0
105.00	203.0
105.80	680.0
106.90	170.0
110.00	150.0
111.00	183.0
111.60	52.0
112.10	135.0
112.90	148.0
114.80	189.0
115.80	459.0
116.90	809.0
118.00	461.0
118.90	909.0
122.80	59.0
123.70	61.0
124.70	75.0
125.30	155.0
126.00	55.0
128.00	464.0
128.80	268.0
129.90	348.0
131.10	229.0
131.90	70.0
133.00	214.0
134.70	137.0
135.20	168.0
135.80	92.0
136.80	187.0
138.90	70.0
139.80	161.0

Instrument :
MSVOA_W
ClientSampleId :
BFB546

140.90	1136.0
141.90	67.0
142.90	1420.0
143.70	96.0
145.20	236.0
146.00	151.0
147.00	68.0
147.90	363.0
150.00	164.0
152.70	50.0
155.10	232.0
156.00	116.0
157.00	326.0
157.90	81.0
159.00	199.0
160.80	168.0
165.10	57.0
167.30	54.0
168.80	62.0
170.70	224.0
172.00	459.0
174.00	73504.0
175.00	5432.0
176.00	73960.0
177.00	4170.0
178.00	215.0
190.90	264.0
192.00	69.0
193.00	244.0
194.10	57.0
207.00	241.0
208.30	62.0
249.00	103.0
260.30	84.0
265.10	114.0
266.20	64.0
267.10	92.0
279.70	63.0
281.20	2134.0
282.00	633.0
283.10	473.0

Instrument :
MSVOA_W
ClientSampleId :
BFB546