

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025834.D
 Acq On : 03 May 2023 18:09
 Operator : SY/MD
 Sample : 02574-20
 Misc : 5.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCQ2

Quant Time: May 04 01:28:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	871104	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	772547	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	355878	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	280892	22.755	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.040%
7) Chloroethane-d5	2.899	69	208019	22.730	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.920%
11) 1,1-Dichloroethene-d2	4.027	65	133514	21.600	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.400%
21) 2-Butanone-d5	7.075	46	175429	42.989	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.980%
24) Chloroform-d	7.648	84	535949	21.337	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.360%
26) 1,2-Dichloroethane-d4	8.471	65	78	0.005	ug/L	0.17
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	1127520	22.336	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.360%
36) 1,2-Dichloropropane-d6	9.270	67	360945	22.348	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.400%
41) Toluene-d8	10.325	98	996953	22.148	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.600%
43) trans-1,3-Dichloroprop...	10.575	79	140441	21.451	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.800%
47) 2-Hexanone-d5	10.922	63	123257	44.754	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	279686	22.720	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.880%
66) 1,2-Dichlorobenzene-d4	13.855	152	306572	23.631	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.520%
Target Compounds						
					Qvalue	
13) Acetone	4.125	43	42100	11.635	ug/L	90
14) Carbon disulfide	4.393	76	26941	0.684	ug/L #	93
16) Methylene chloride	4.917	84	56783	3.161	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
Data File : VW025834.D
Acq On : 03 May 2023 18:09
Operator : SY/MD
Sample : 02574-20
Misc : 5.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCQ2

Quant Time: May 04 01:28:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 04 01:22:04 2023
Response via : Initial Calibration




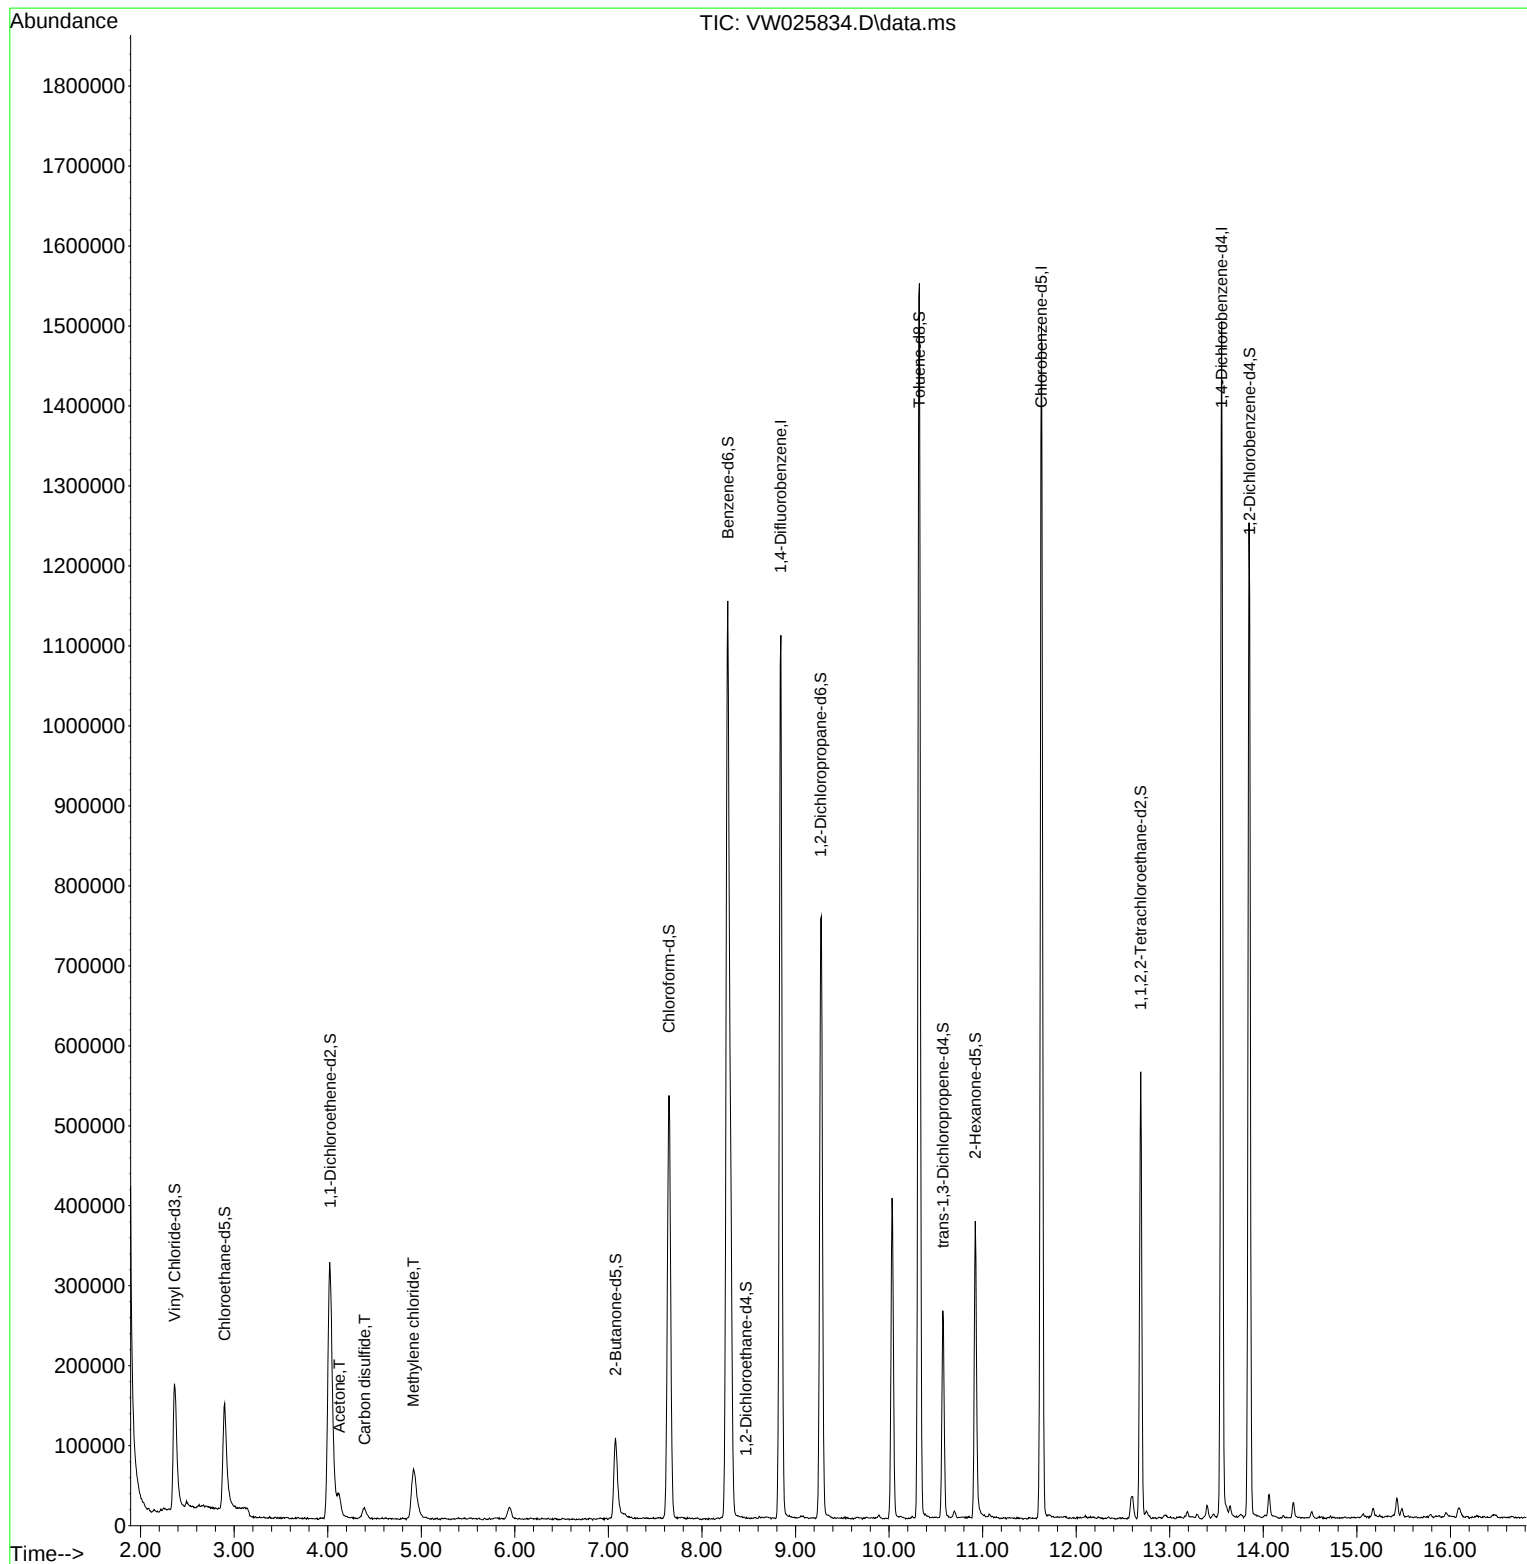


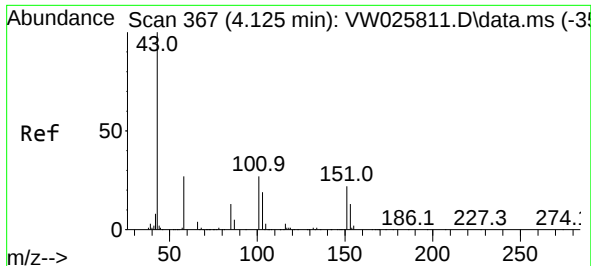

#13
Acetone
Concen: 11.635 ug/L
RT: 4.125 min Scan# 367
Delta R.T. 0.000 min
Lab File: VW025834.D
Acq: 03 May 2023 18:09




Instrument :
MSVOA_W
ClientSampleId :
DCCQ2


Tgt Ion: 43 Resp: 42100
Ion Ratio Lower Upper
43 100
58 34.4 0.0 58.2

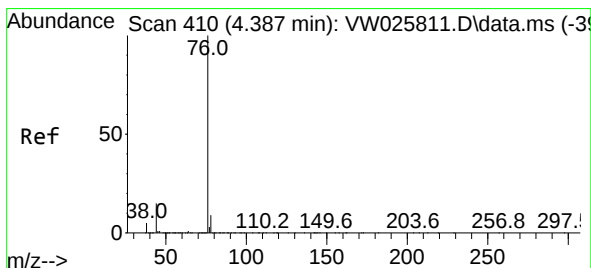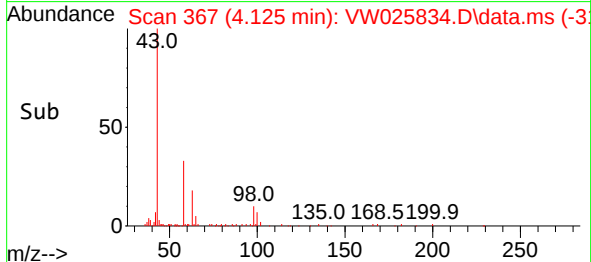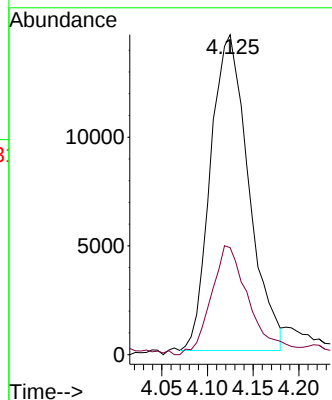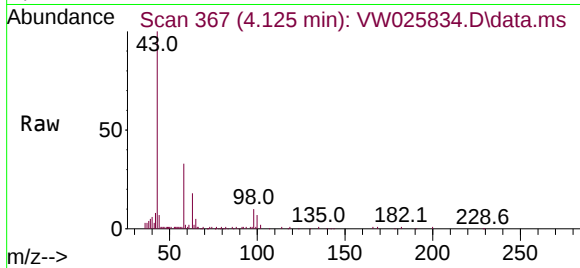

#14
Carbon disulfide
Concen: 0.684 ug/L
RT: 4.393 min Scan# 411
Delta R.T. 0.006 min
Lab File: VW025834.D
Acq: 03 May 2023 18:09

Tgt Ion: 76 Resp: 26941
Ion Ratio Lower Upper
76 100
78 11.7 7.4 11.0#

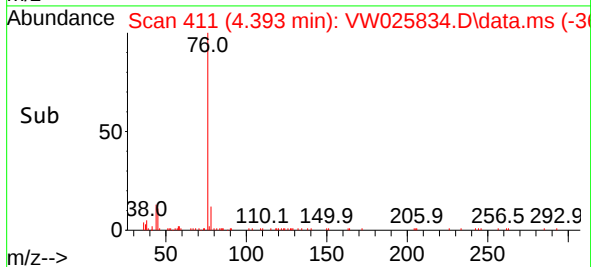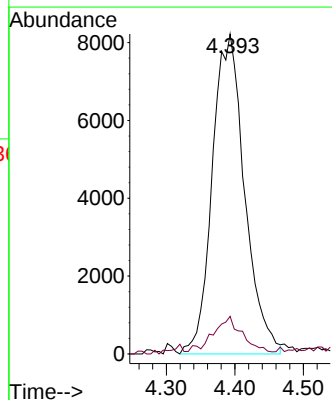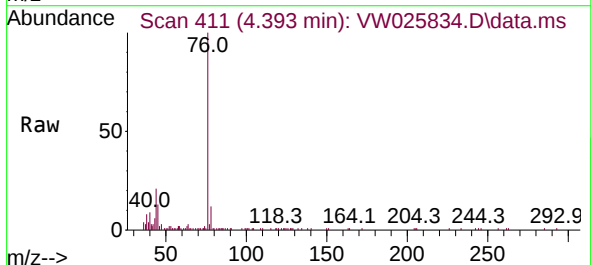

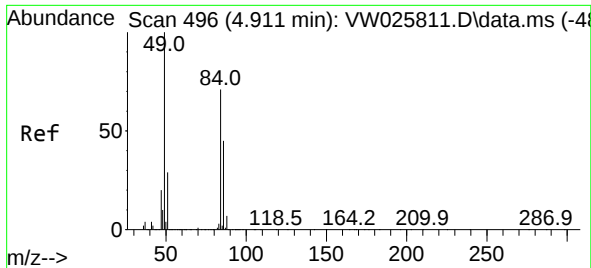

#16
Methylene chloride
Concen: 3.161 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW025834.D
Acq: 03 May 2023 18:09

Instrument :
MSVOA_W
ClientSampleId :
DCCQ2

Tgt Ion: 84 Resp: 56783
Ion Ratio Lower Upper
84 100
86 64.2 41.7 77.5
49 144.9 95.3 177.1

