




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025818.D
 Acq On : 03 May 2023 11:45
 Operator : SY/MD
 Sample : 02574-11
 Misc : 3.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCS6

Manual IntegrationsAPPROVED

Quant Time: May 04 01:24:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

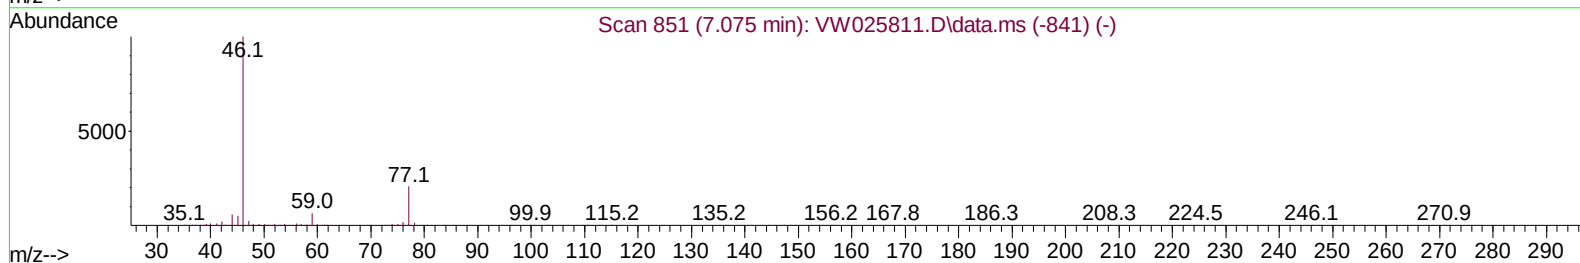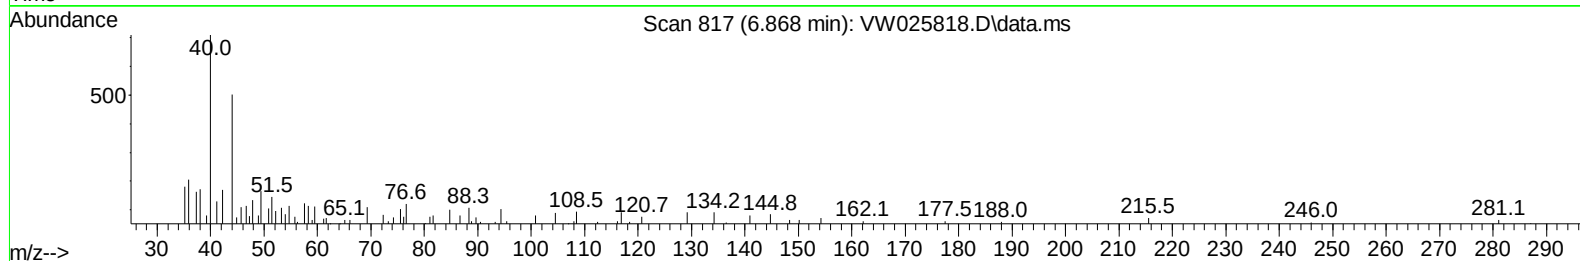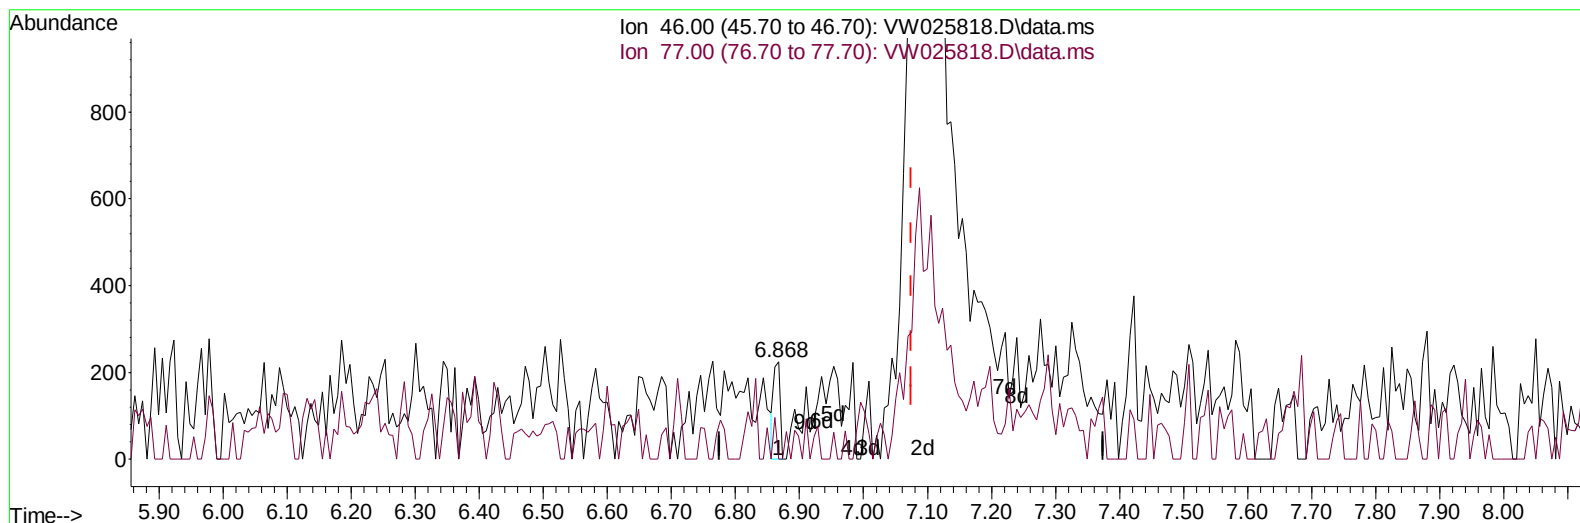

TIC: VW025818.D\data.ms

(21) 2-Butanone-d5 (S)

6.868min (-0.207) 0.66 ug/L

response 160

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.00	22.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025818.D
 Acq On : 03 May 2023 11:45
 Operator : SY/MD
 Sample : 02574-11
 Misc : 3.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCS6

Manual IntegrationsAPPROVED

Quant Time: May 04 01:24:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

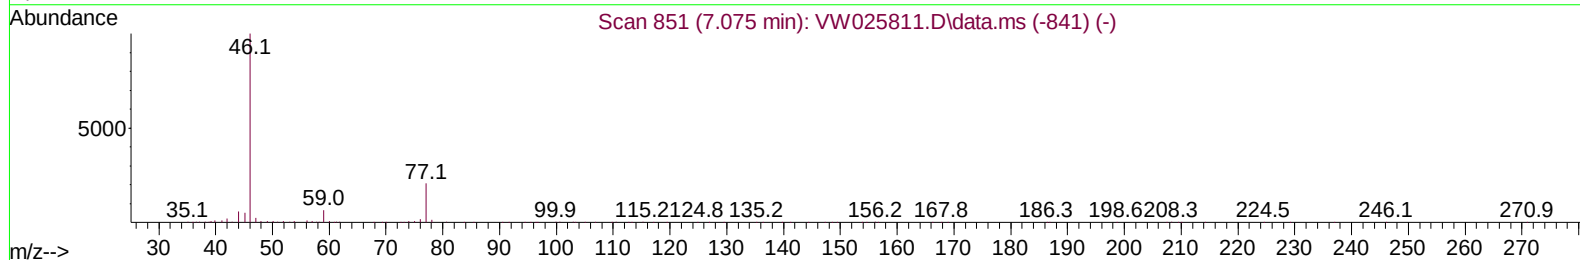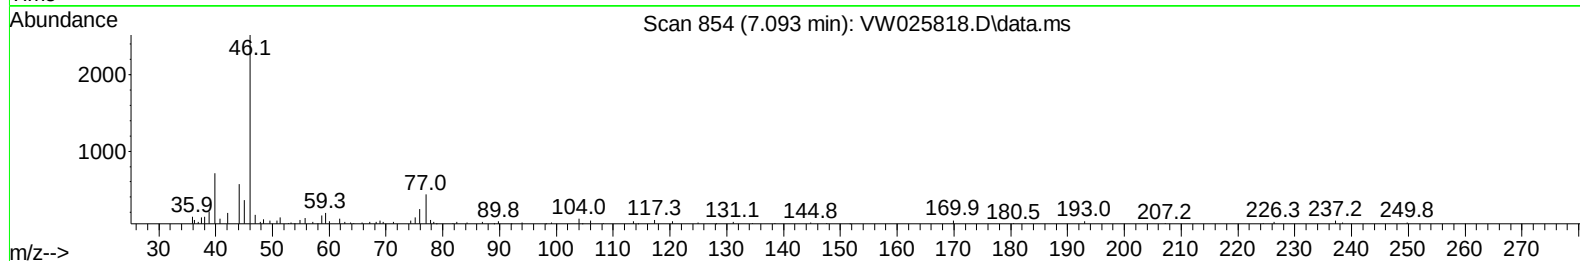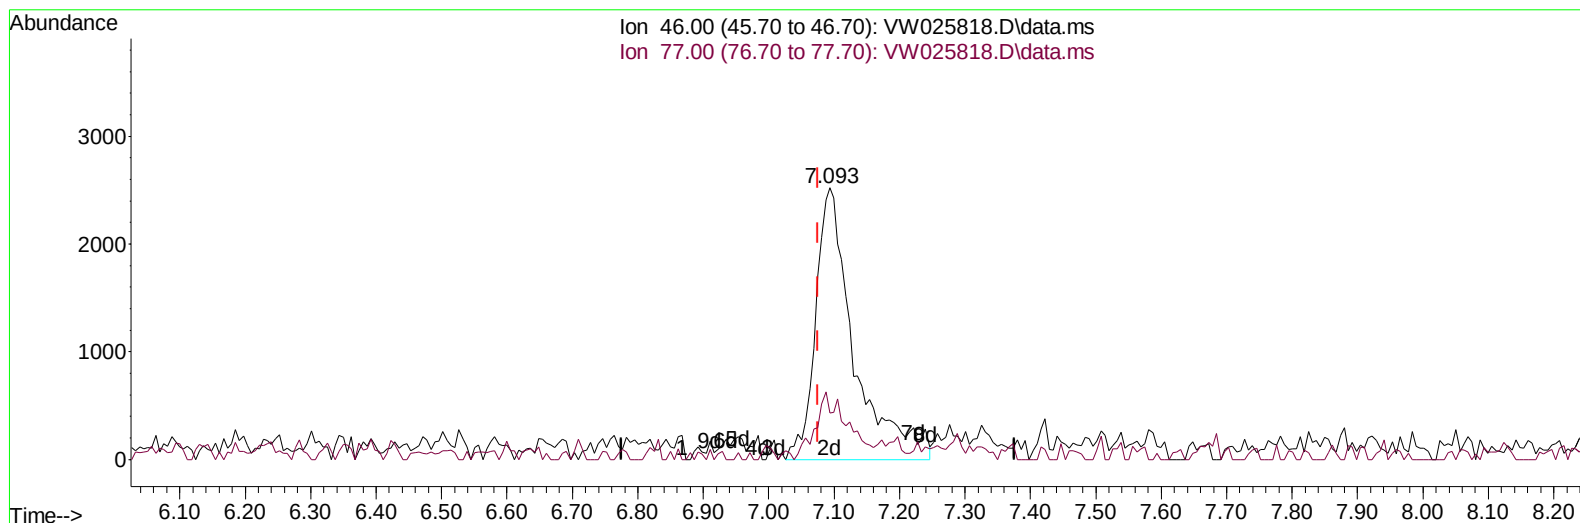

TIC: VW025818.D\data.ms

(21) 2-Butanone-d5 (S)

7.093min (+ 0.018) 42.32 ug/L m

response 10254

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.00	0.35#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025818.D
 Acq On : 03 May 2023 11:45
 Operator : SY/MD
 Sample : 02574-11
 Misc : 3.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCS6

Manual IntegrationsAPPROVED

Quant Time: May 04 01:24:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	51717	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	47088	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	20171	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	17330	23.647	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.600%	
7) Chloroethane-d5	2.887	69	15522	28.569	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	114.280%	
11) 1,1-Dichloroethene-d2	4.027	65	8245	22.468	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	89.880%	
21) 2-Butanone-d5	7.093	46	10254m	42.324	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	84.640%	
24) Chloroform-d	7.654	84	30714	20.596	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.400%	
26) 1,2-Dichloroethane-d4	8.313	65	18433	21.859	ug/L	0.01
Spiked Amount 25.000	Range 70	- 130	Recovery	=	87.440%	
32) Benzene-d6	8.276	84	61588	20.017	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.080%	
36) 1,2-Dichloropropane-d6	9.270	67	19893	20.207	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	80.840%	
41) Toluene-d8	10.325	98	45972	16.756	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	67.040%	
43) trans-1,3-Dichloroprop...	10.581	79	7136	17.883	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.520%	
47) 2-Hexanone-d5	10.928	63	4539	27.039	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	54.080%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	16537	22.040	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	88.160%	
66) 1,2-Dichlorobenzene-d4	13.848	152	14721	20.020	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	80.080%	
Target Compounds						
16) Methylene chloride	4.929	84	2232	2.093	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
Data File : VW025818.D
Acq On : 03 May 2023 11:45
Operator : SY/MD
Sample : 02574-11
Misc : 3.82g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCS6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2023
Supervised By :Mahesh Dadoda 05/04/2023

Quant Time: May 04 01:24:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 04 01:22:04 2023
Response via : Initial Calibration

