




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025825.D
 Acq On : 03 May 2023 14:33
 Operator : SY/MD
 Sample : 02574-07
 Misc : 5.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCP2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

Quant Time: May 04 01:26:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

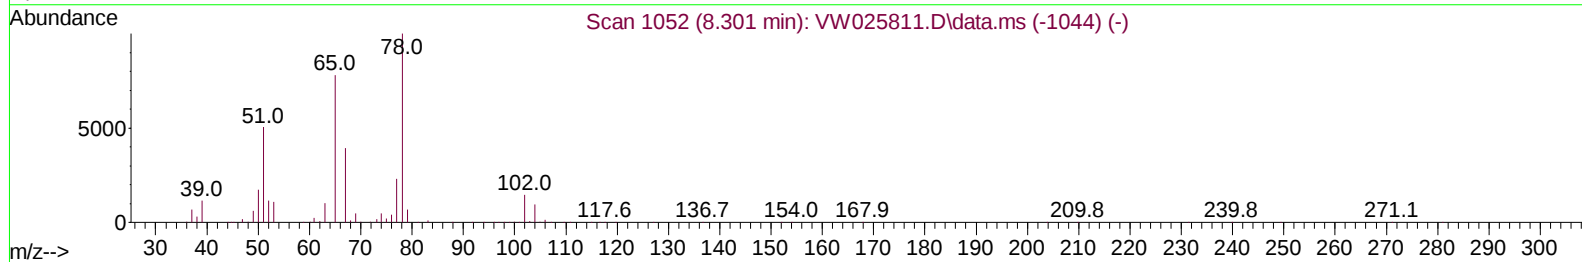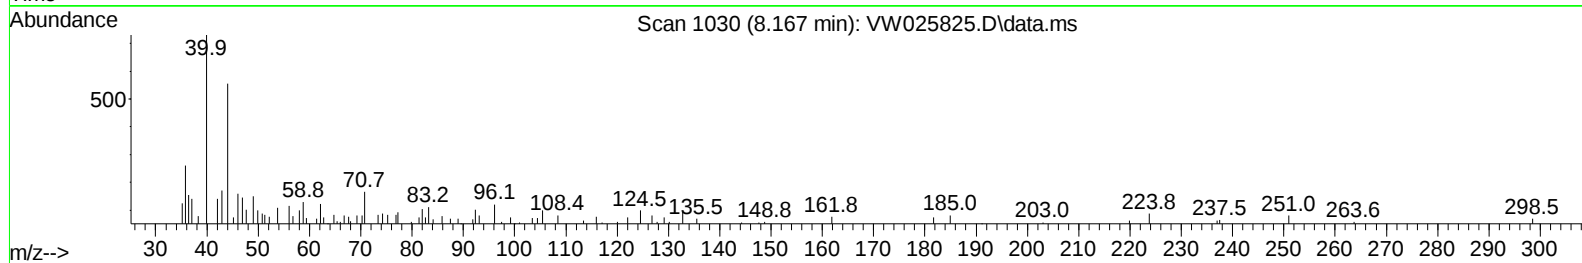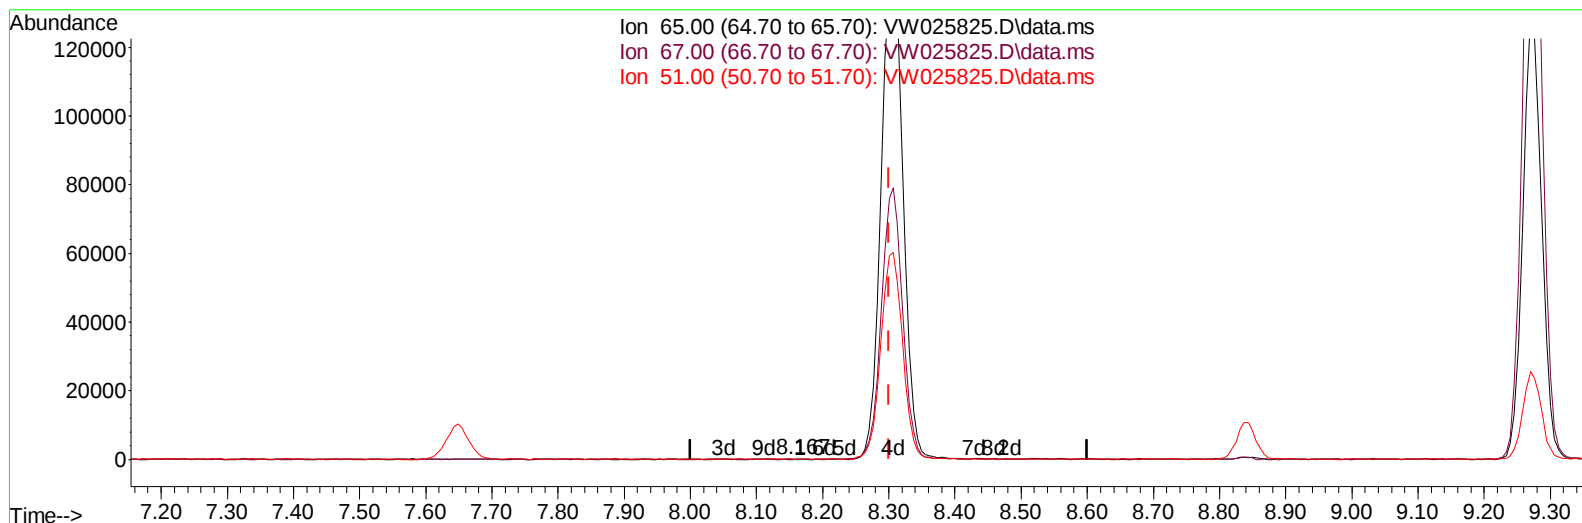

TIC: VW025825.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.167min (-0.134) 0.01 ug/L

response 157

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	53.50
51.00	112.30	88.54
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025825.D
 Acq On : 03 May 2023 14:33
 Operator : SY/MD
 Sample : 02574-07
 Misc : 5.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCP2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

Quant Time: May 04 01:26:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

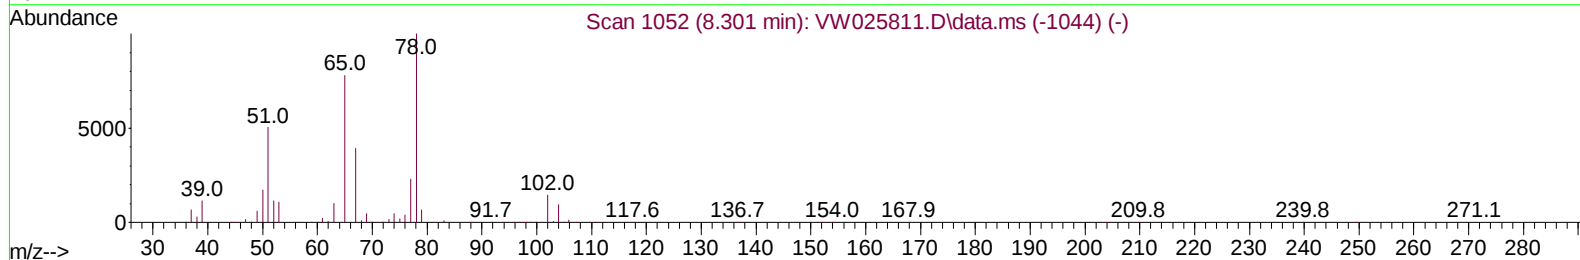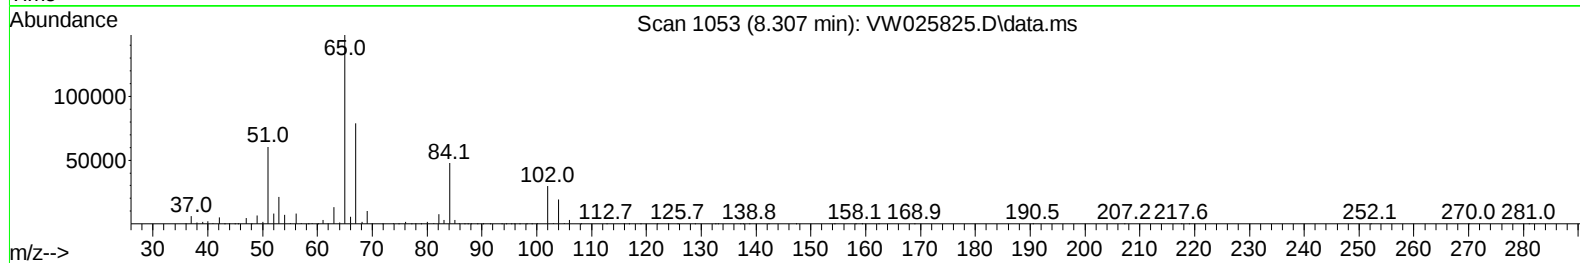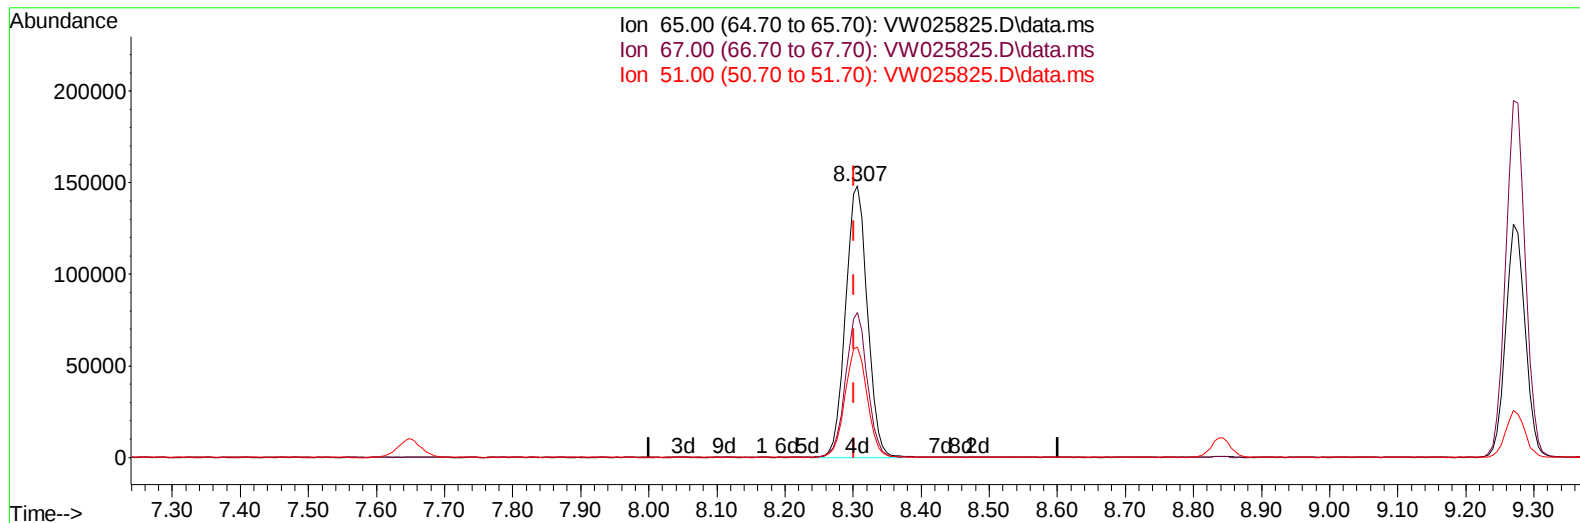

TIC: VW025825.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 21.53 ug/L m

response 332970

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.03#
51.00	112.30	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025825.D
 Acq On : 03 May 2023 14:33
 Operator : SY/MD
 Sample : 02574-07
 Misc : 5.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCP2

Manual IntegrationsAPPROVED

Quant Time: May 04 01:26:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	948378	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	842058	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	375966	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	316625	23.560	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.240%	
7) Chloroethane-d5	2.899	69	231867	23.272	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	93.080%	
11) 1,1-Dichloroethene-d2	4.021	65	147647	21.940	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	87.760%	
21) 2-Butanone-d5	7.075	46	179065	40.304	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	80.600%	
24) Chloroform-d	7.648	84	584697	21.381	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	85.520%	
26) 1,2-Dichloroethane-d4	8.307	65	332970m	21.532	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	86.120%	
32) Benzene-d6	8.270	84	1229507	22.346	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	89.400%	
36) 1,2-Dichloropropane-d6	9.270	67	391984	22.266	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	89.080%	
41) Toluene-d8	10.319	98	1076373	21.938	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.760%	
43) trans-1,3-Dichloroprop...	10.575	79	147259	20.636	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	82.560%	
47) 2-Hexanone-d5	10.922	63	123377	41.100	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	82.200%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	283950	21.162	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	84.640%	
66) 1,2-Dichlorobenzene-d4	13.848	152	330546	24.118	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.480%	
Target Compounds						
					Qvalue	
13) Acetone	4.119	43	108055	27.429	ug/L	99
16) Methylene chloride	4.917	84	34206	1.749	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
Data File : VW025825.D
Acq On : 03 May 2023 14:33
Operator : SY/MD
Sample : 02574-07
Misc : 5.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCP2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2023
Supervised By :Mahesh Dadoda 05/04/2023

Quant Time: May 04 01:26:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 04 01:22:04 2023
Response via : Initial Calibration

