




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025829.D
 Acq On : 03 May 2023 16:09
 Operator : SY/MD
 Sample : 02574-05
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCP0

Manual IntegrationsAPPROVED

Quant Time: May 04 01:27:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

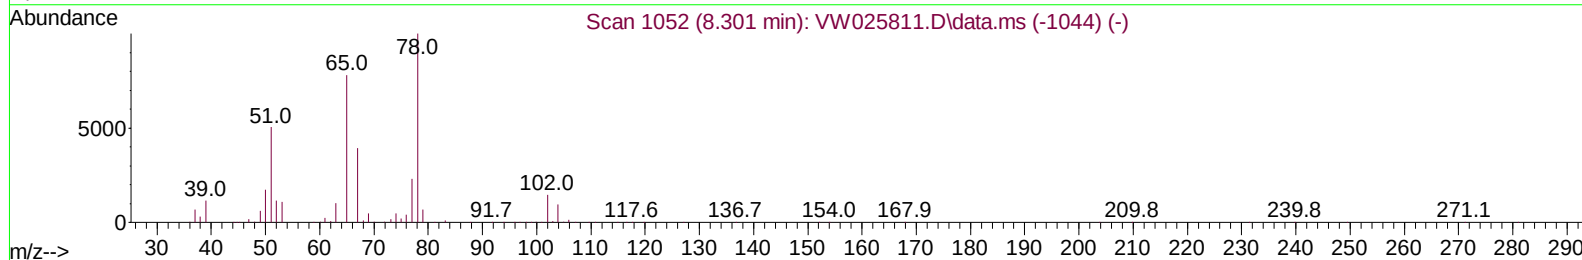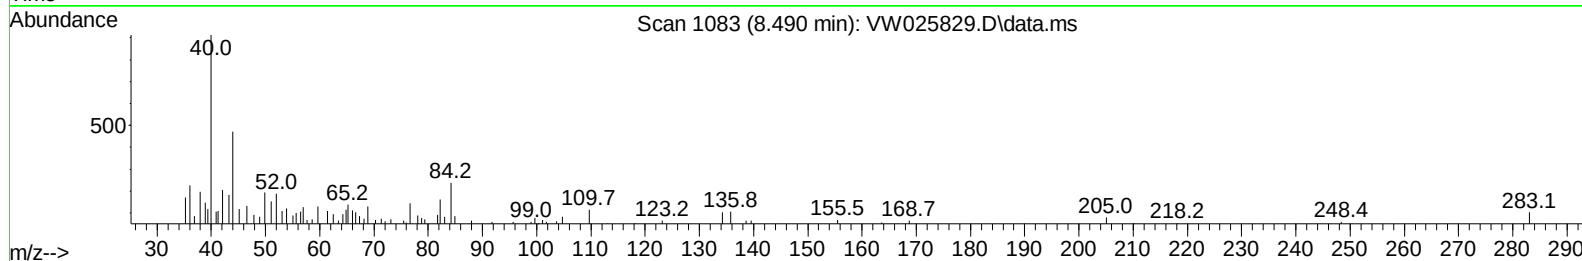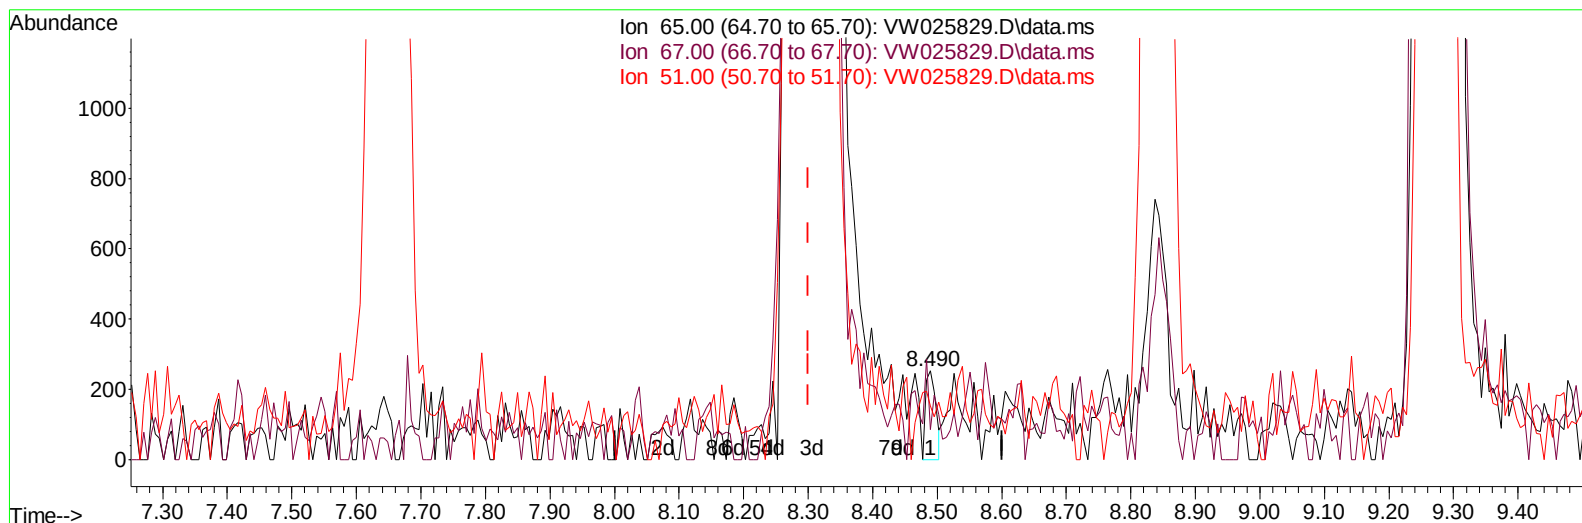

TIC: VW025829.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.490min (+ 0.189) 0.02 ug/L

response 277

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	42.24
51.00	112.30	120.94
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025829.D
 Acq On : 03 May 2023 16:09
 Operator : SY/MD
 Sample : 02574-05
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCP0

Manual IntegrationsAPPROVED

Quant Time: May 04 01:27:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

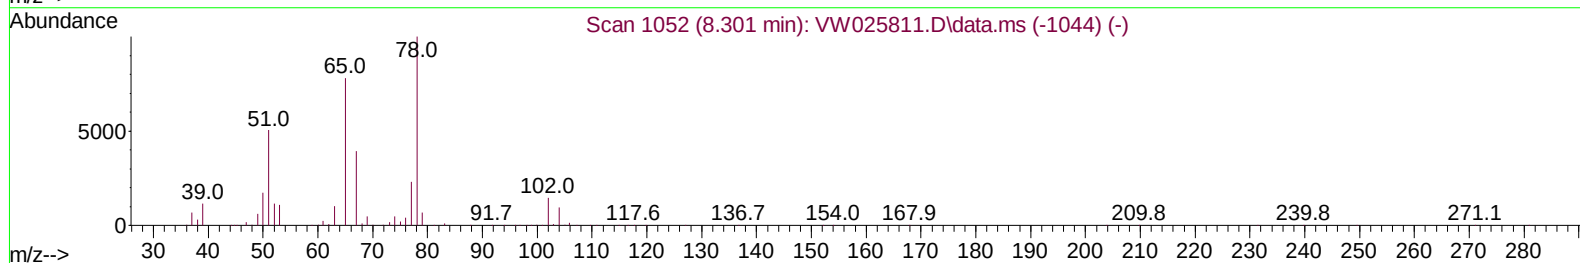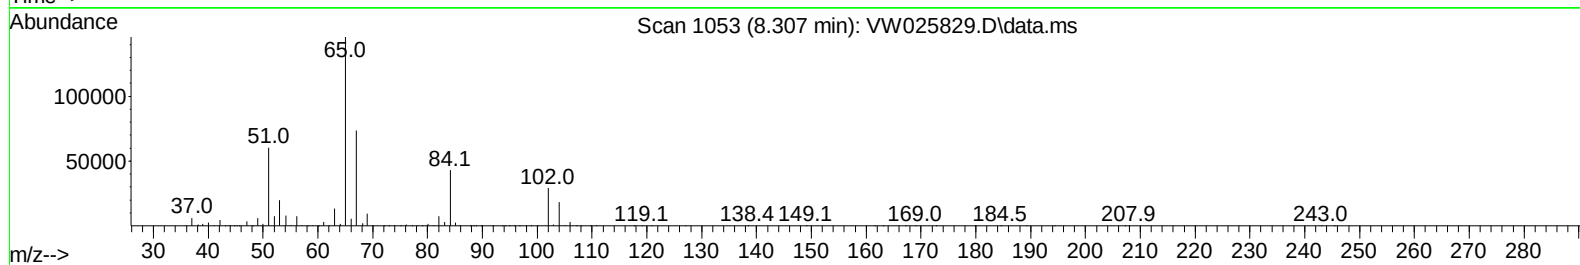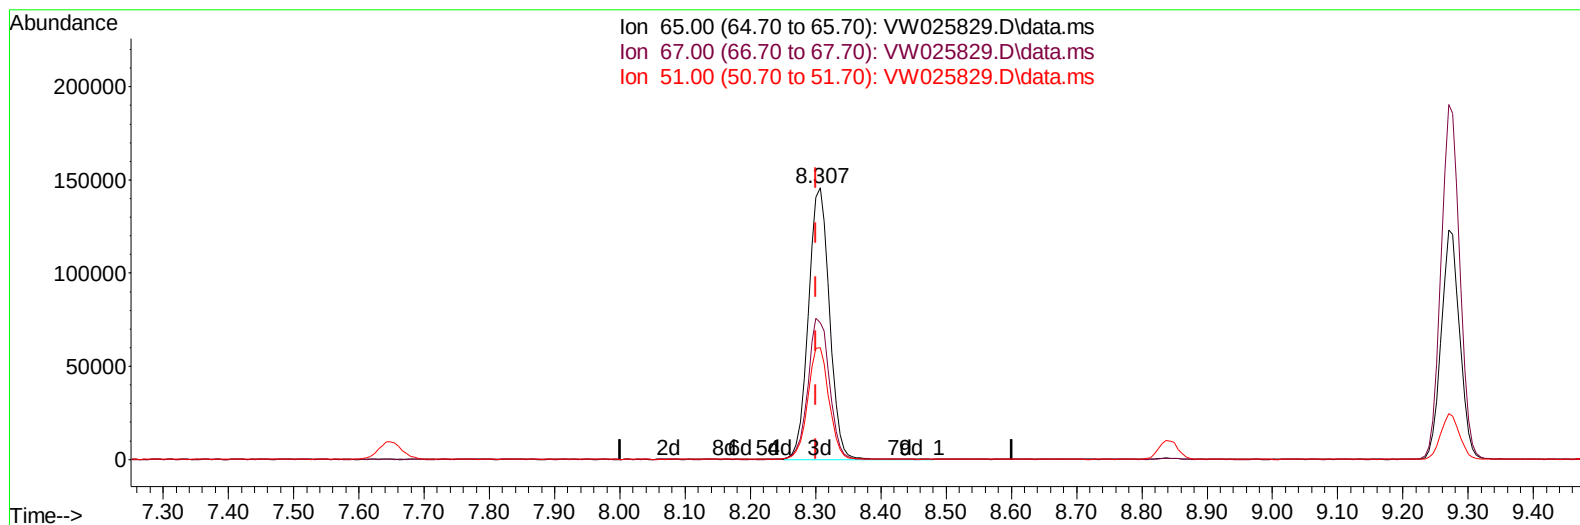

TIC: VW025829.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 22.21 ug/L m

response 326484

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.04#
51.00	112.30	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025829.D
 Acq On : 03 May 2023 16:09
 Operator : SY/MD
 Sample : 02574-05
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCP0

Manual IntegrationsAPPROVED

Quant Time: May 04 01:27:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/04/2023
 Supervised By :Mahesh Dadoda 05/04/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		901541	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		800817	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		364623	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		303651	23.768	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.080%	
7) Chloroethane-d5	2.893	69		221842	23.422	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.680%	
11) 1,1-Dichloroethene-d2	4.027	65		141780	22.163	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	88.640%	
21) 2-Butanone-d5	7.075	46		179981	42.615	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	85.240%	
24) Chloroform-d	7.648	84		560587	21.564	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	86.240%	
26) 1,2-Dichloroethane-d4	8.307	65		326484m	22.210	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	88.840%	
32) Benzene-d6	8.276	84		1153456	22.043	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	88.160%	
36) 1,2-Dichloropropane-d6	9.270	67		378511	22.608	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	90.440%	
41) Toluene-d8	10.325	98		1031843	22.114	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	88.440%	
43) trans-1,3-Dichloroprop...	10.575	79		141823	20.898	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	83.600%	
47) 2-Hexanone-d5	10.922	63		124148	43.486	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	86.980%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		281085	22.027	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	88.120%	
66) 1,2-Dichlorobenzene-d4	13.848	152		301638	22.693	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	90.760%	
Target Compounds							
						Qvalue	
13) Acetone	4.119	43		110908	29.616	ug/L	100
16) Methylene chloride	4.917	84		31886	1.715	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
Data File : VW025829.D
Acq On : 03 May 2023 16:09
Operator : SY/MD
Sample : 02574-05
Misc : 5.33g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCP0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/04/2023
Supervised By :Mahesh Dadoda 05/04/2023

Quant Time: May 04 01:27:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 04 01:22:04 2023
Response via : Initial Calibration

