

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
 Data File : VW025813.D
 Acq On : 03 May 2023 09:45
 Operator : SY/MD
 Sample : 02549-11
 Misc : 5.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCCC8

Quant Time: May 04 01:23:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 04 01:22:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	849324	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	764725	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	350132	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	282855	23.502	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.000%
7) Chloroethane-d5	2.899	69	209660	23.497	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.000%
11) 1,1-Dichloroethene-d2	4.021	65	136665	22.677	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.720%
21) 2-Butanone-d5	7.075	46	182397	45.842	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.680%
24) Chloroform-d	7.648	84	512824	20.940	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.760%
26) 1,2-Dichloroethane-d4	8.307	65	305363	22.050	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.200%
32) Benzene-d6	8.276	84	1075751	21.528	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.120%
36) 1,2-Dichloropropane-d6	9.276	67	347510	21.736	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.960%
41) Toluene-d8	10.324	98	958942	21.521	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.080%
43) trans-1,3-Dichloroprop...	10.574	79	134946	20.823	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.280%
47) 2-Hexanone-d5	10.922	63	125341	45.976	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.960%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	274068	22.491	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.960%
66) 1,2-Dichlorobenzene-d4	13.848	152	295467	23.149	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.600%
Target Compounds					Qvalue	
13) Acetone	4.118	43	107643	30.511	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050323\
Data File : VW025813.D
Acq On : 03 May 2023 09:45
Operator : SY/MD
Sample : 02549-11
Misc : 5.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCCC8

Quant Time: May 04 01:23:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 04 01:22:04 2023
Response via : Initial Calibration

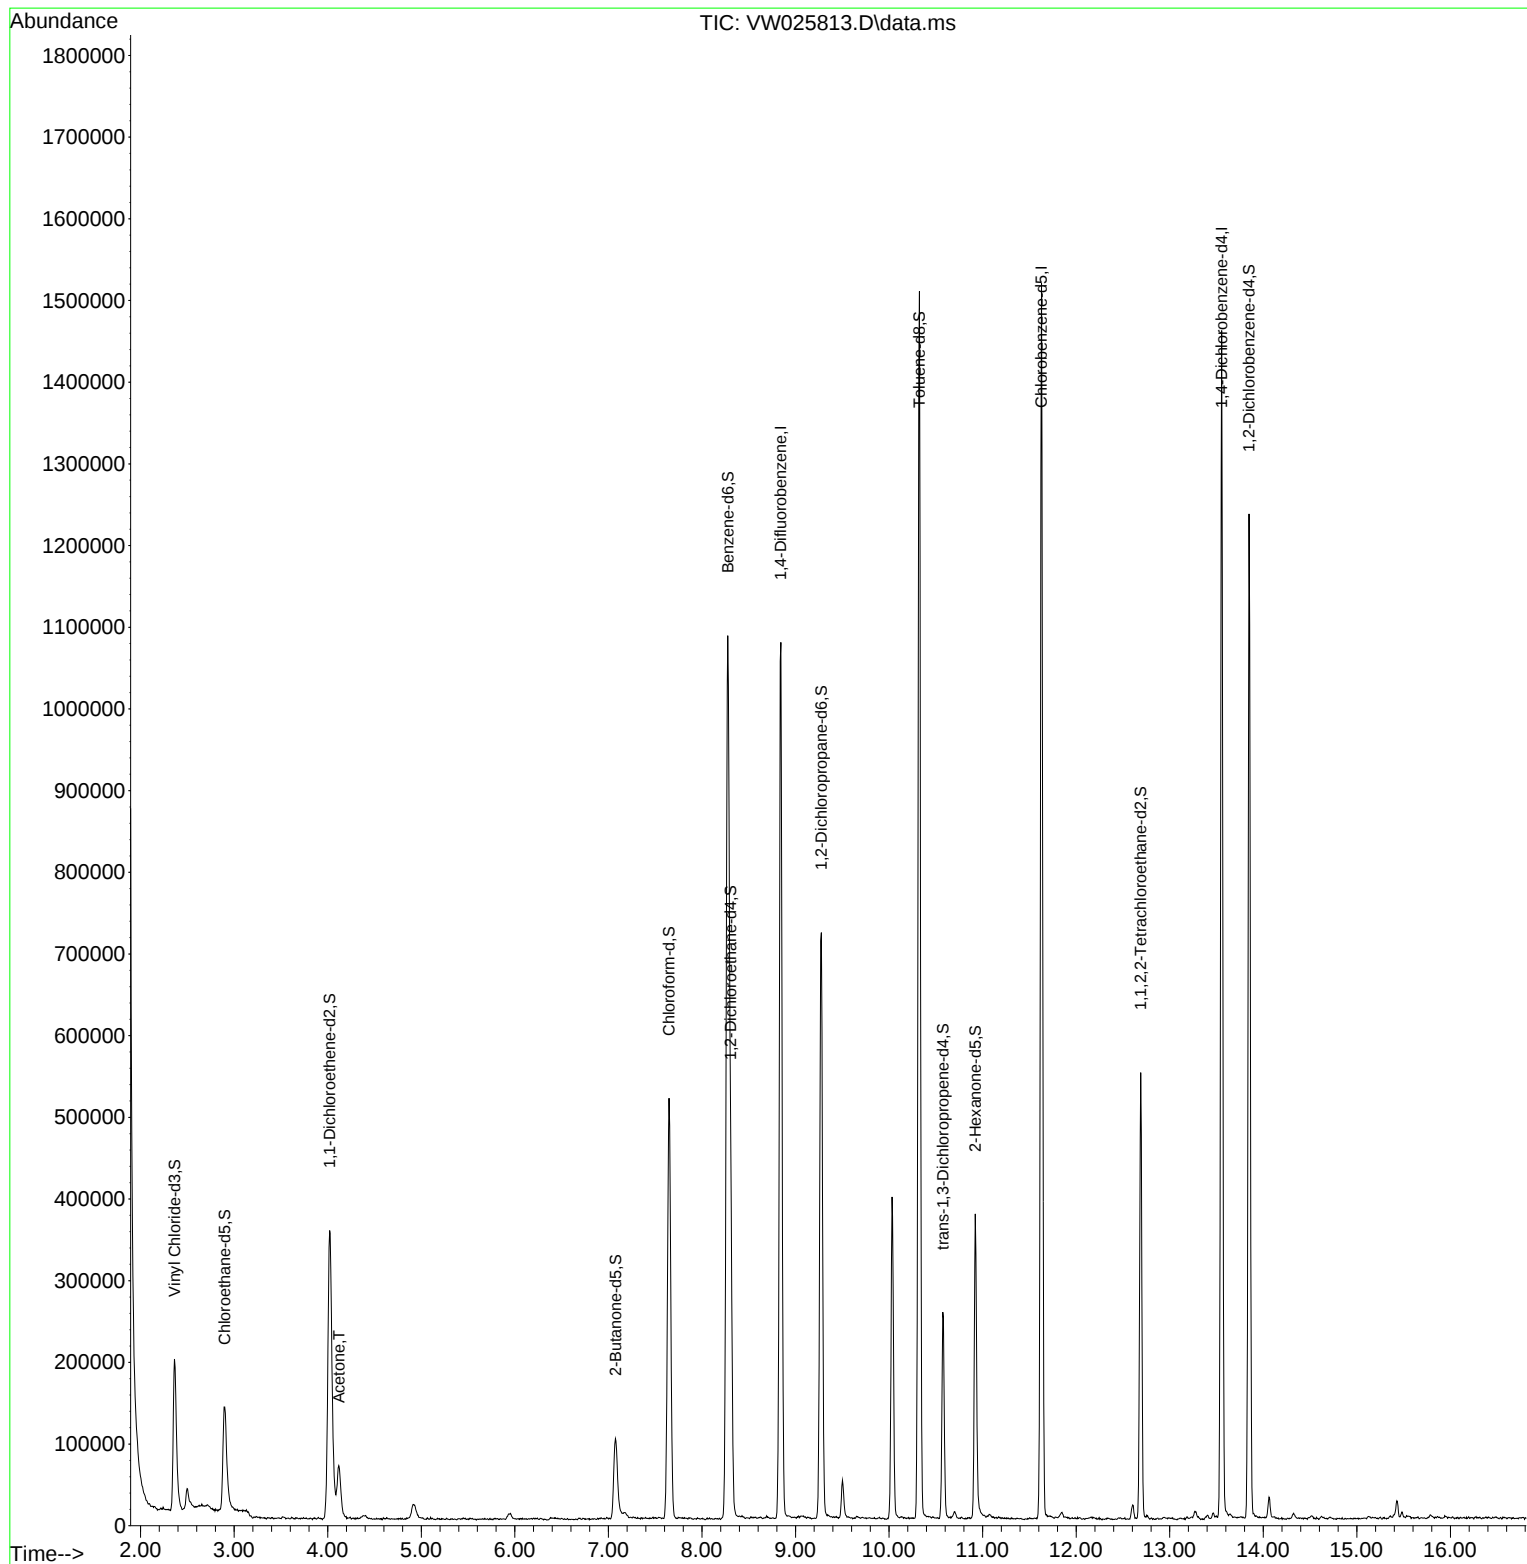

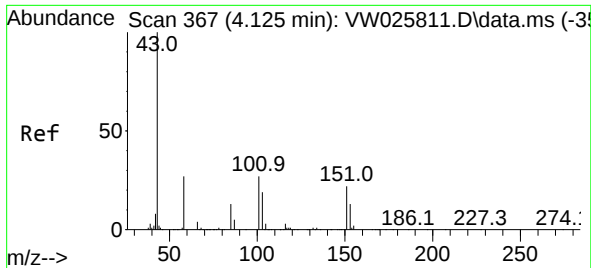

#13

Acetone

Concen: 30.511 ug/L

RT: 4.118 min Scan# 30

Delta R.T. -0.006 min

Lab File: VW025813.D


Acq: 03 May 2023 09:45

Instrument :

MSVOA_W

ClientSampleId :

DCCC8

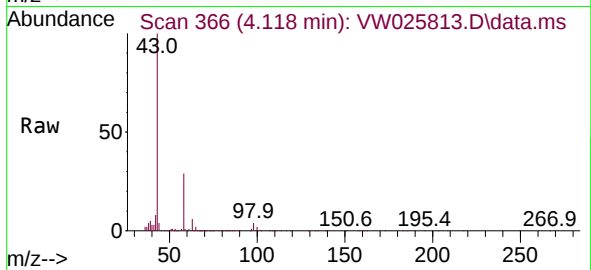

Tgt Ion: 43 Resp: 107643

Ion Ratio Lower Upper

43 100

58 29.5 0.0 58.2

