


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050420\
 Data File : VW015382.D
 Acq On : 04 May 2020 11:58
 Operator : SY/VA
 Sample : BFB27
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB27

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM050420S.M
 Title : VOC Analysis
 Last Update : Mon May 04 15:08:09 2020

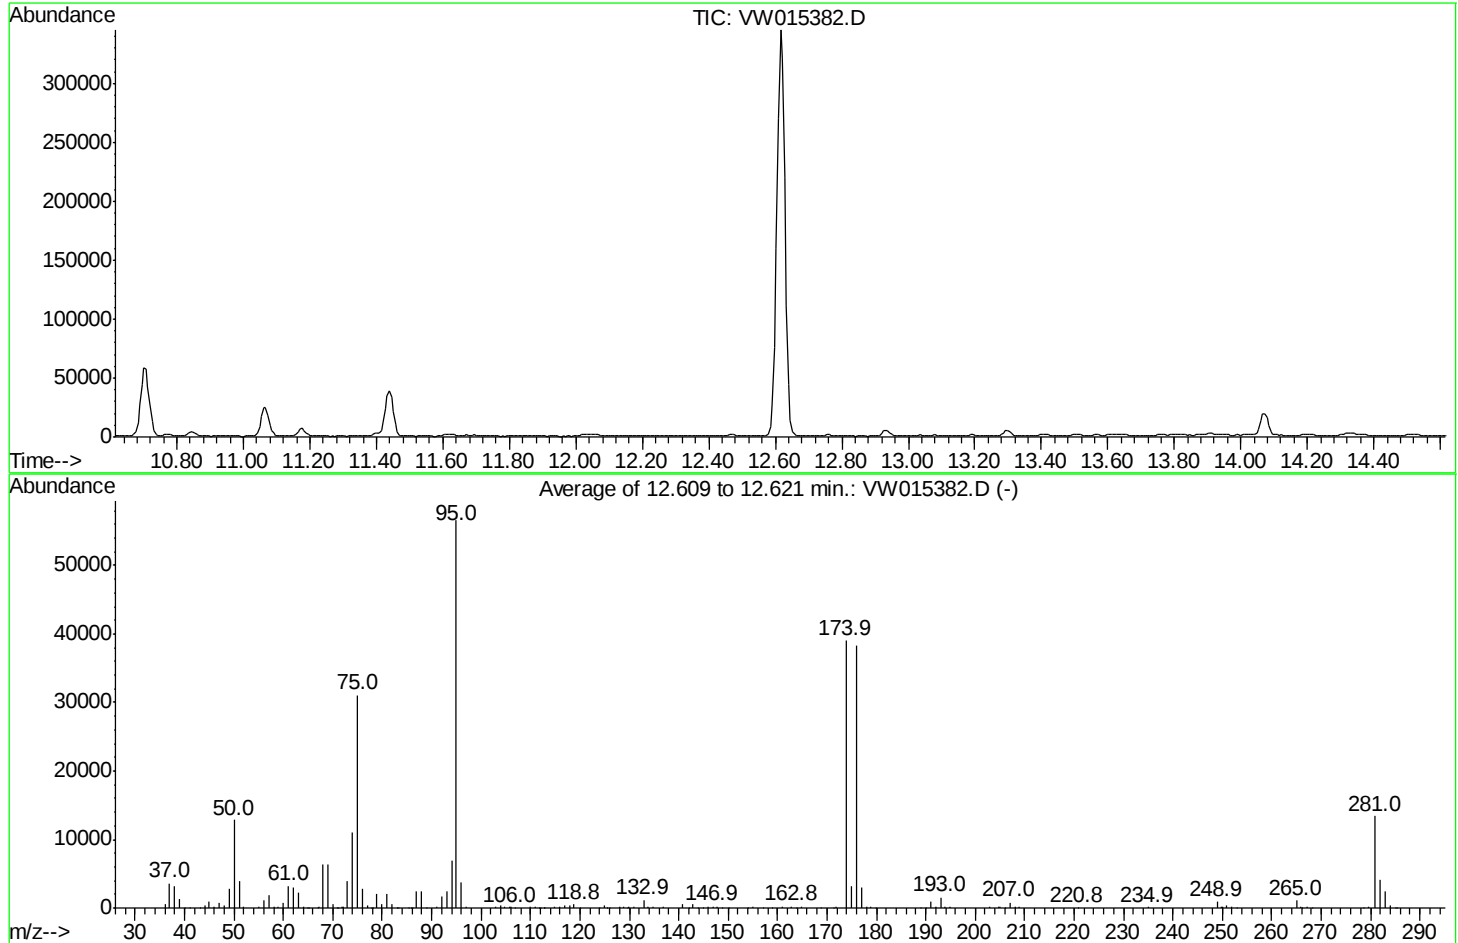

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	12850	PASS
75	95	30	80	54.9	31090	PASS
95	95	100	100	100.0	56589	PASS
96	95	5	9	6.8	3828	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.0	39026	PASS
175	174	5	9	8.2	3184	PASS
176	174	95	101	98.3	38365	PASS
177	176	5	9	7.8	2984	PASS

m/z	Abundance
36.00	582.0
37.00	3155.0
38.00	2754.0
39.00	1097.0
39.90	141.0
40.90	124.0
43.00	185.0
44.10	690.0
45.00	929.0
46.00	131.0
47.00	735.0
47.90	366.0
49.00	2262.0
50.00	11285.0
51.00	3695.0
52.00	157.0
54.90	215.0
56.00	1006.0
57.00	1649.0
58.00	132.0
59.00	296.0
60.00	606.0
61.00	2904.0
62.00	2635.0
63.00	1897.0
64.00	187.0
64.90	51.0
66.90	207.0
68.00	5503.0
69.00	5358.0
70.00	441.0
70.80	77.0
71.90	317.0
73.00	4099.0
74.00	9310.0
75.00	26360.0
76.00	2339.0
77.00	371.0
78.90	1761.0
79.90	578.0
81.00	1776.0
81.90	447.0
82.90	55.0
85.20	51.0
86.90	2214.0
87.90	2077.0
89.00	70.0
90.90	240.0
92.00	1400.0
93.00	1963.0
94.00	5736.0
95.00	46416.0
96.00	3368.0
96.90	126.0
102.90	396.0
103.90	317.0
104.80	178.0
105.80	221.0
106.00	223.0
106.90	77.0
109.90	143.0
111.10	135.0
112.00	101.0
112.70	61.0
115.00	168.0
115.80	207.0
116.90	467.0
118.00	412.0
118.80	460.0
120.00	66.0
125.00	539.0
128.00	165.0
128.90	99.0
129.70	136.0
130.00	122.0
130.90	170.0
132.90	1676.0
134.80	184.0
136.90	79.0
140.90	475.0
142.90	431.0
143.90	64.0
145.90	109.0
146.90	327.0
147.80	148.0
148.80	94.0
150.00	85.0
154.80	131.0
156.90	62.0
160.80	174.0
162.90	316.0
163.90	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB27

164.90	234.0
168.70	65.0
171.90	103.0
173.90	28056.0
174.90	2287.0
175.90	27384.0
176.90	2400.0
177.90	224.0
178.90	400.0
179.90	59.0
189.10	116.0
189.90	58.0
191.00	1420.0
191.90	317.0
193.00	1897.0
193.90	370.0
194.90	258.0
202.90	116.0
204.80	368.0
207.00	1136.0
208.00	294.0
209.10	99.0
220.80	85.0
235.00	184.0
248.90	1142.0
249.80	361.0
251.00	549.0
251.90	221.0
252.80	78.0
265.00	1449.0
265.90	278.0
267.00	261.0
268.10	61.0
278.70	137.0
281.00	16672.0
282.00	5431.0
283.00	3486.0
284.00	543.0
285.20	193.0

Instrument :
MSVOA_W
ClientSampleId :
BFB27

m/z	Abundance
36.00	731.0
37.00	3958.0
38.00	3573.0
39.00	1393.0
39.90	207.0
41.00	104.0
42.10	72.0
43.00	164.0
44.00	760.0
45.00	929.0
46.10	142.0
46.90	766.0
47.90	437.0
49.00	3289.0
50.00	14270.0
51.00	4253.0
52.00	233.0
55.00	324.0
56.00	1243.0
57.00	2141.0
58.10	181.0
59.00	285.0
60.00	813.0
61.00	3827.0
62.00	3337.0
63.00	2488.0
64.00	254.0
64.80	61.0
65.20	51.0
67.10	241.0
68.00	7226.0
69.00	7230.0
70.00	495.0
71.00	50.0
71.90	448.0
73.00	4372.0
74.00	12275.0
75.00	34424.0
76.00	3151.0
76.90	386.0
77.80	240.0
78.90	2175.0
79.90	631.0
80.90	2458.0
81.90	507.0
83.20	77.0
85.90	100.0
87.00	2690.0
87.90	2694.0
90.90	289.0
92.00	2033.0
93.00	2765.0
94.00	7599.0
95.00	62960.0
96.00	4127.0
97.00	128.0
103.00	218.0
103.90	438.0
104.80	193.0
105.90	269.0
106.90	98.0
109.80	136.0
110.90	133.0
111.70	110.0
112.90	57.0
114.90	194.0
115.90	266.0
116.90	415.0
117.90	422.0
118.90	599.0
124.00	66.0
124.90	465.0
126.10	83.0
127.90	275.0
128.80	111.0
129.90	223.0
130.80	129.0
133.00	1236.0
133.80	184.0
134.80	202.0
136.90	91.0
140.80	527.0
142.00	91.0
142.90	645.0
144.80	105.0
145.90	142.0
147.00	193.0
147.80	213.0
148.90	67.0
149.80	83.0
154.00	70.0
154.90	113.0

Instrument :
MSVOA_W
ClientSampleId :
BFB27

157.00	95.0
158.90	86.0
160.90	142.0
162.80	202.0
165.00	231.0
168.70	60.0
171.20	78.0
171.80	154.0
173.90	41912.0
175.00	3641.0
175.90	43416.0
176.90	3483.0
178.00	233.0
179.00	310.0
188.90	86.0
191.00	1023.0
192.00	234.0
193.00	1765.0
194.00	228.0
195.00	197.0
203.00	166.0
205.00	268.0
206.00	64.0
207.00	839.0
208.00	135.0
209.00	159.0
220.80	70.0
235.00	155.0
249.00	950.0
250.00	220.0
250.90	358.0
252.00	134.0
252.90	81.0
265.00	1058.0
265.90	317.0
267.10	326.0
278.60	101.0
279.60	156.0
281.00	14183.0
282.10	4049.0
283.00	2435.0
284.00	457.0
284.90	174.0

Instrument :
MSVOA_W
ClientSampleId :
BFB27

m/z	Abundance
36.00	621.0
37.00	3728.0
38.00	3276.0
39.00	1231.0
40.00	211.0
40.80	62.0
43.10	108.0
44.00	764.0
45.00	701.0
46.10	66.0
46.90	661.0
47.90	455.0
49.00	3009.0
50.00	12996.0
51.00	3676.0
52.00	206.0
55.10	201.0
56.00	1243.0
57.00	1961.0
58.00	93.0
59.00	112.0
60.00	609.0
61.00	3087.0
62.00	3229.0
63.00	2442.0
64.00	259.0
65.10	69.0
67.10	156.0
68.00	6527.0
69.00	6514.0
69.90	527.0
72.10	314.0
73.00	3328.0
74.00	11361.0
75.00	32488.0
76.00	2753.0
77.00	363.0
78.10	278.0
78.90	2042.0
79.90	579.0
80.90	2195.0
81.90	534.0
83.10	85.0
86.10	95.0
86.90	2349.0
87.90	2410.0
91.00	232.0
92.00	1902.0
93.00	2654.0
94.00	7441.0
95.00	60392.0
96.00	3991.0
96.90	181.0
102.80	160.0
103.80	293.0
104.90	161.0
105.80	242.0
106.90	55.0
109.90	106.0
110.80	92.0
112.00	72.0
115.00	159.0
116.00	195.0
116.90	339.0
117.80	319.0
118.90	416.0
124.00	70.0
124.90	255.0
125.50	107.0
126.10	52.0
127.90	212.0
128.90	108.0
129.90	197.0
130.80	108.0
133.00	621.0
133.80	183.0
134.80	204.0
136.90	135.0
140.90	494.0
142.00	120.0
142.90	632.0
144.90	81.0
145.90	74.0
146.80	119.0
147.90	151.0
148.90	62.0
150.00	83.0
155.00	117.0
156.90	133.0
159.00	73.0
161.00	124.0
162.80	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB27

165.00	109.0
168.70	69.0
171.70	141.0
173.90	47112.0
174.90	3626.0
176.00	44296.0
176.90	3070.0
177.90	113.0
178.90	133.0
188.90	93.0
190.90	436.0
192.00	218.0
193.00	855.0
194.00	168.0
195.00	61.0
202.80	80.0
205.00	131.0
206.90	456.0
207.90	95.0
208.90	61.0
234.80	83.0
249.00	643.0
249.90	169.0
250.90	240.0
264.90	659.0
266.10	106.0
267.00	192.0
279.60	146.0
281.00	9492.0
282.10	2602.0
283.00	1393.0
283.90	213.0
285.00	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB27

Scan 1749 (12.566 min): VW015382.D
BFB27

m/z	Abundance
40.00	184.0
41.20	66.0
41.90	51.0
43.10	80.0
43.90	349.0
57.30	63.0
68.80	94.0
99.80	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB27