

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022793.D
 Acq On : 04 May 2022 11:40
 Operator : SY/VA
 Sample : N2632-05RE
 Misc : 6.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A6RE

Quant Time: May 04 23:35:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	255311	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	225203	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	83605	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	121745	23.242	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.960%
7) Chloroethane-d5	2.885	69	82730	24.277	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.120%
11) 1,1-Dichloroethene-d2	4.019	63	110686	16.354	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.400%
21) 2-Butanone-d5	7.080	46	51768	51.980	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.960%
24) Chloroform-d	7.647	84	178657	23.885	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.520%
26) 1,2-Dichloroethane-d4	8.567	65	124	0.030	ug/L	0.26
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.275	84	339994	26.193	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.760%
36) 1,2-Dichloropropane-d6	9.274	67	99982	27.420	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.680%
41) Toluene-d8	10.323	98	299483	23.884	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.520%
43) trans-1,3-Dichloroprop...	10.579	79	38128	22.710	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.840%
47) 2-Hexanone-d5	10.921	63	41931	60.240	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.480%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	94934	27.933	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.720%
66) 1,2-Dichlorobenzene-d4	13.853	152	73856	25.271	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.080%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	3493	0.702	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022793.D
Acq On : 04 May 2022 11:40
Operator : SY/VA
Sample : N2632-05RE
Misc : 6.81g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4A6RE

Quant Time: May 04 23:35:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

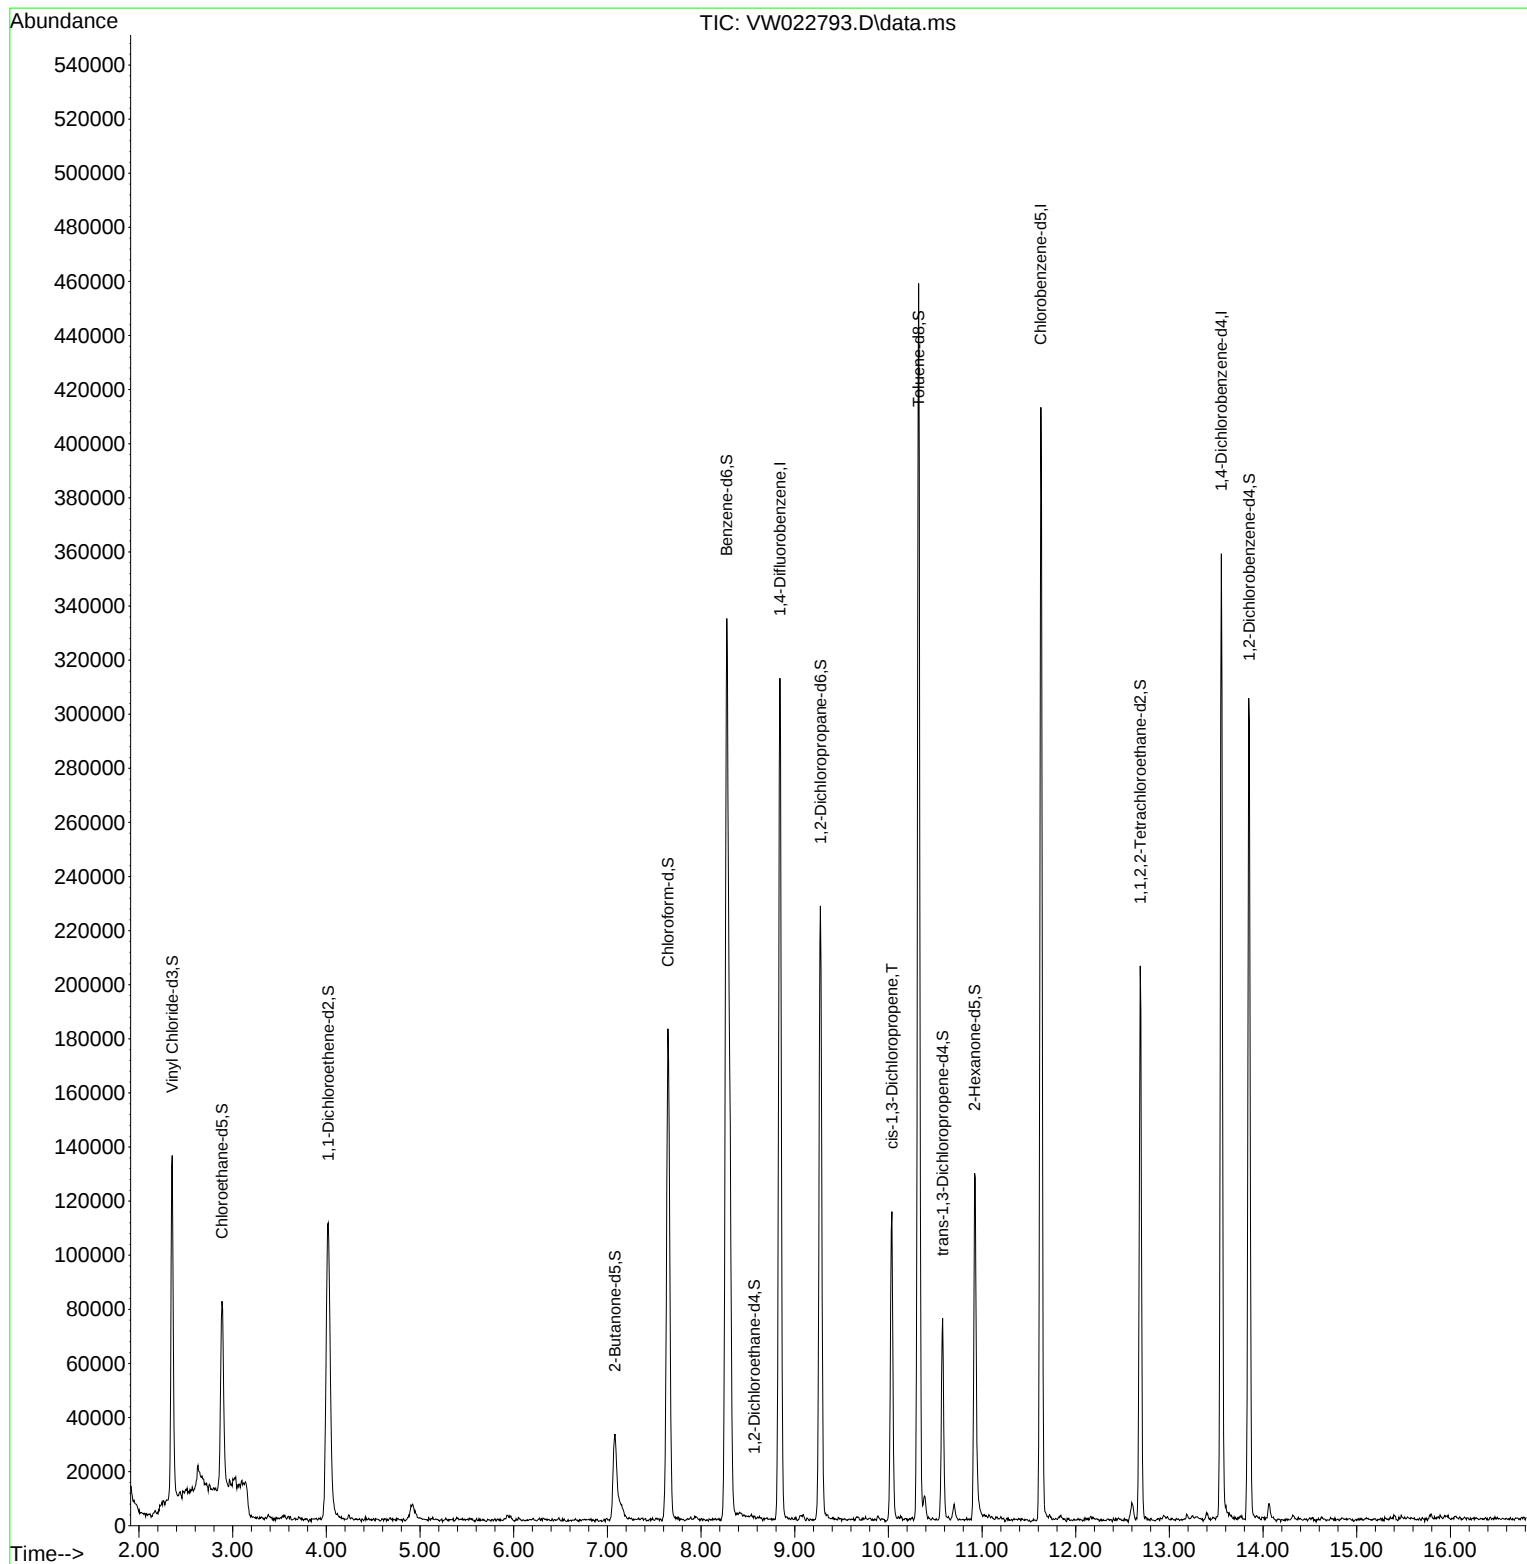

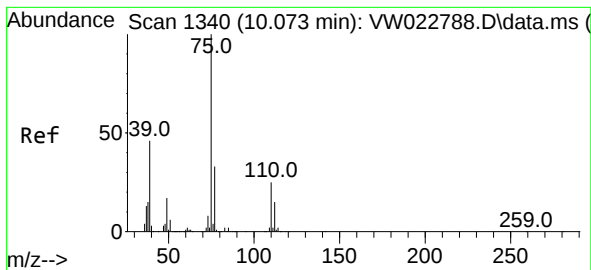

#39
 cis-1,3-Dichloropropene
 Concen: 0.702 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022793.D
 Acq: 04 May 2022 11:40

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A6RE

Tgt Ion: 75 Resp: 3493
 Ion Ratio Lower Upper
 75 100
 77 39.2 22.1 41.1

