

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022818.D
 Acq On : 04 May 2022 22:38
 Operator : SY/VA
 Sample : N2699-04
 Misc : 4.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBQ7

Quant Time: May 05 02:59:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	263849	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	222822	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77779	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	108574	20.057	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.240%
7) Chloroethane-d5	2.885	69	83528	23.718	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.880%
11) 1,1-Dichloroethene-d2	4.019	63	104577	14.951	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.800%
21) 2-Butanone-d5	7.080	46	39726	38.598	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.200%
24) Chloroform-d	7.653	84	178955	23.150	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	8.305	65	107305	25.310	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.240%
32) Benzene-d6	8.275	84	323143	25.160	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.640%
36) 1,2-Dichloropropane-d6	9.274	67	104425	28.945	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.760%
41) Toluene-d8	10.323	98	276338	22.273	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.080%
43) trans-1,3-Dichloroprop...	10.579	79	32160	19.360	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.440%
47) 2-Hexanone-d5	10.927	63	29637	43.033	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.060%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	91122	27.098	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.400%
66) 1,2-Dichlorobenzene-d4	13.847	152	59524	21.893	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.560%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	17908	4.638	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022818.D
Acq On : 04 May 2022 22:38
Operator : SY/VA
Sample : N2699-04
Misc : 4.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGBQ7


Quant Time: May 05 02:59:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 05 02:23:51 2022
Response via : Initial Calibration

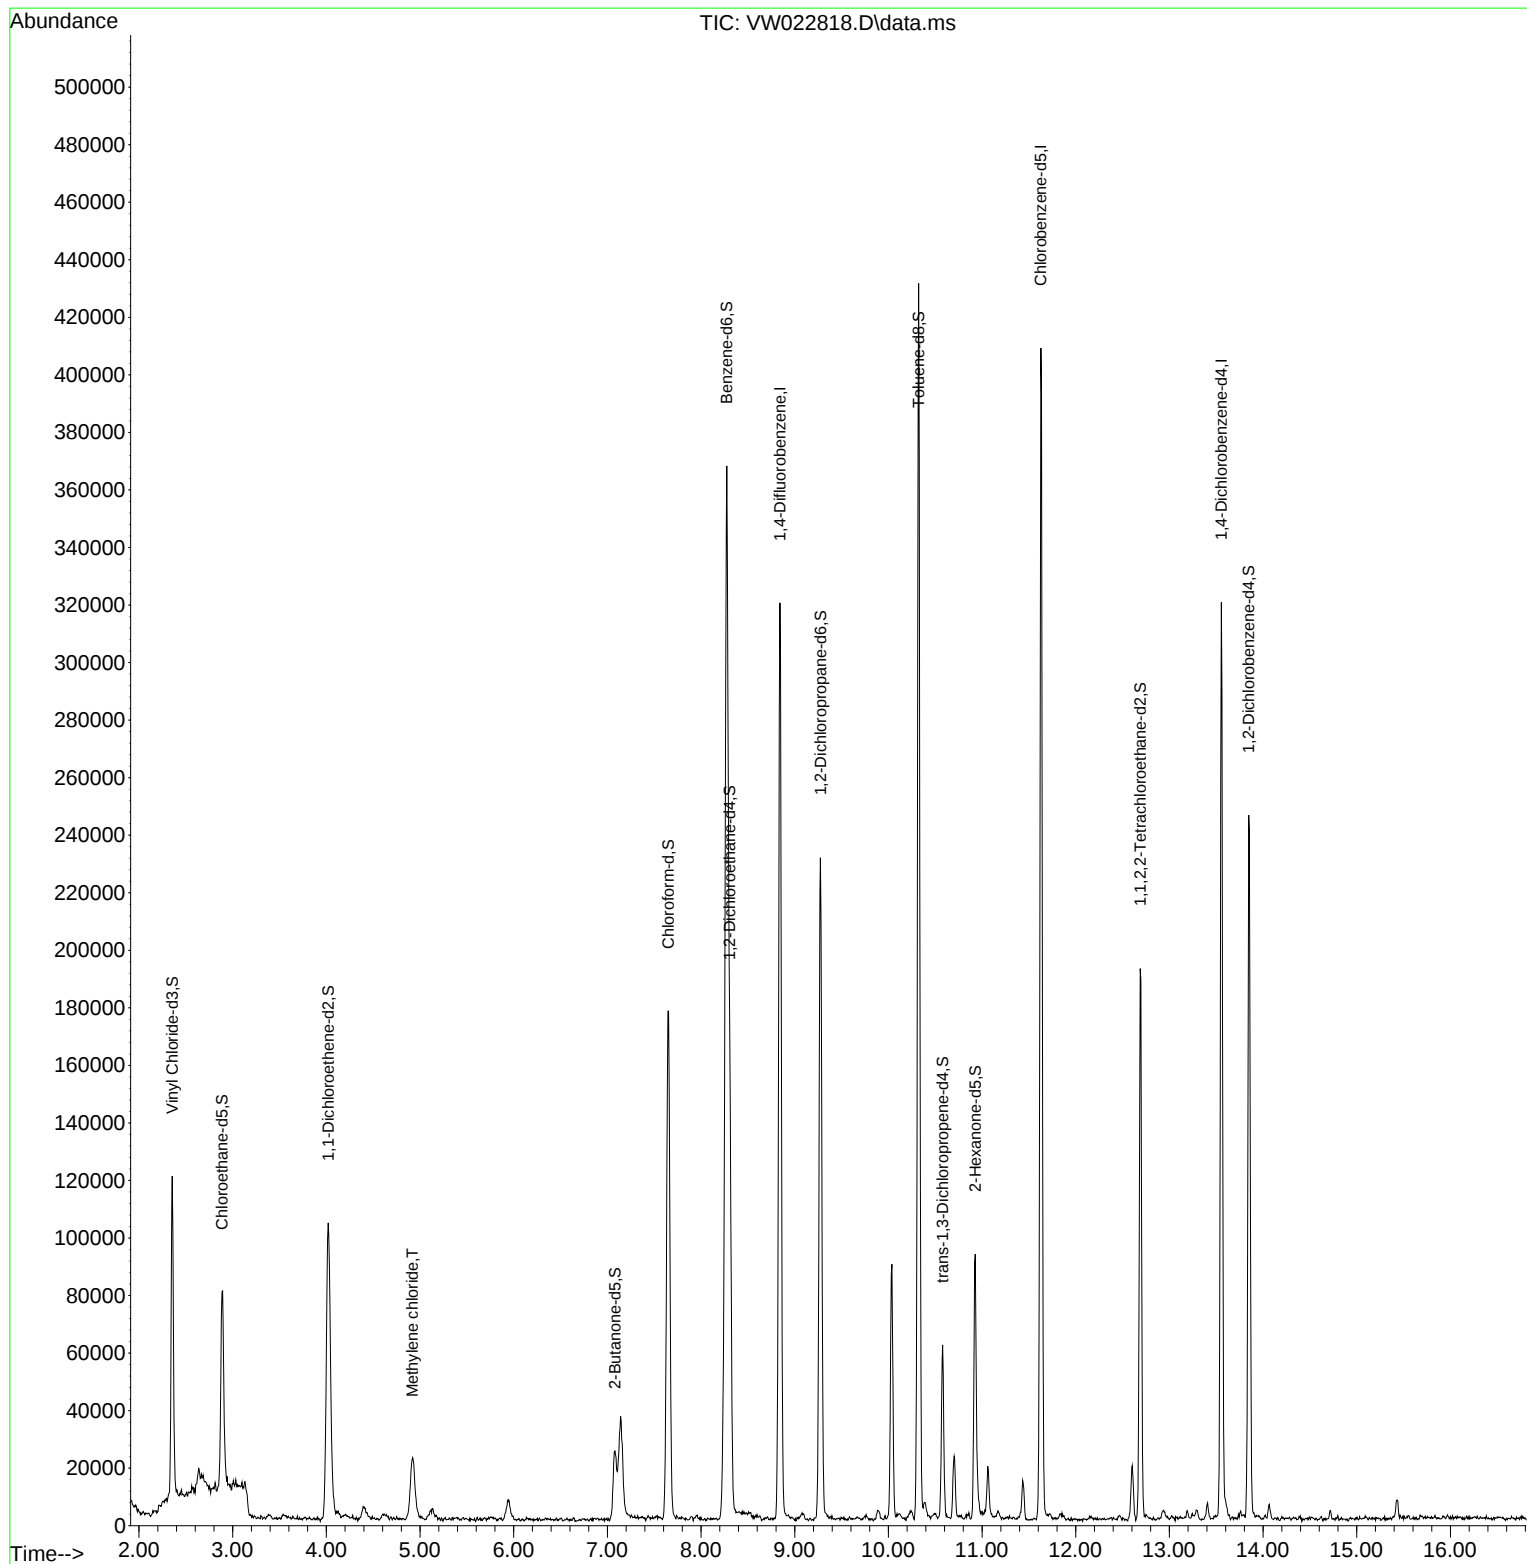

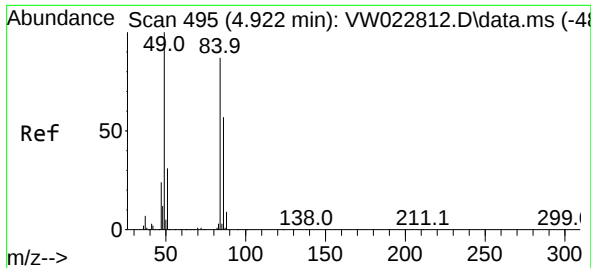

#16
Methylene chloride
Concen: 4.638 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW022818.D
Acq: 04 May 2022 22:38

Instrument :
MSVOA_W
ClientSampleId :
BGBQ7

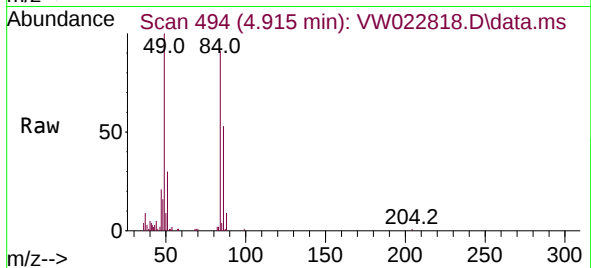

Tgt Ion: 84 Resp: 17908

Ion	Ratio	Lower	Upper
84	100		
86	58.8	45.4	84.4
49	110.2	82.5	153.1

