

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022820.D
 Acq On : 04 May 2022 23:26
 Operator : SY/VA
 Sample : N2699-06
 Misc : 4.76g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGBQ9

Quant Time: May 05 03:00:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 05 02:23:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	297659	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	253976	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	94269	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	119205	19.520	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.080%
7) Chloroethane-d5	2.885	69	88531	22.283	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.120%
11) 1,1-Dichloroethene-d2	4.013	63	112116	14.208	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.840%
21) 2-Butanone-d5	7.073	46	34459	29.677	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.360%
24) Chloroform-d	7.647	84	198606	22.774	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.080%
26) 1,2-Dichloroethane-d4	8.305	65	114795	24.001	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.000%
32) Benzene-d6	8.274	84	367104	25.077	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.320%
36) 1,2-Dichloropropane-d6	9.274	67	112732	27.414	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.640%
41) Toluene-d8	10.323	98	313708	22.184	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.720%
43) trans-1,3-Dichloroprop...	10.573	79	32723	17.283	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.120%
47) 2-Hexanone-d5	10.926	63	28018	35.692	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.380%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	96339	25.135	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	77004	23.368	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.480%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	3521	0.627	ug/L	96
48) 2-Hexanone	10.926	43	3473	2.278	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022820.D
Acq On : 04 May 2022 23:26
Operator : SY/VA
Sample : N2699-06
Misc : 4.76g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGBQ9

Quant Time: May 05 03:00:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 05 02:23:51 2022
Response via : Initial Calibration

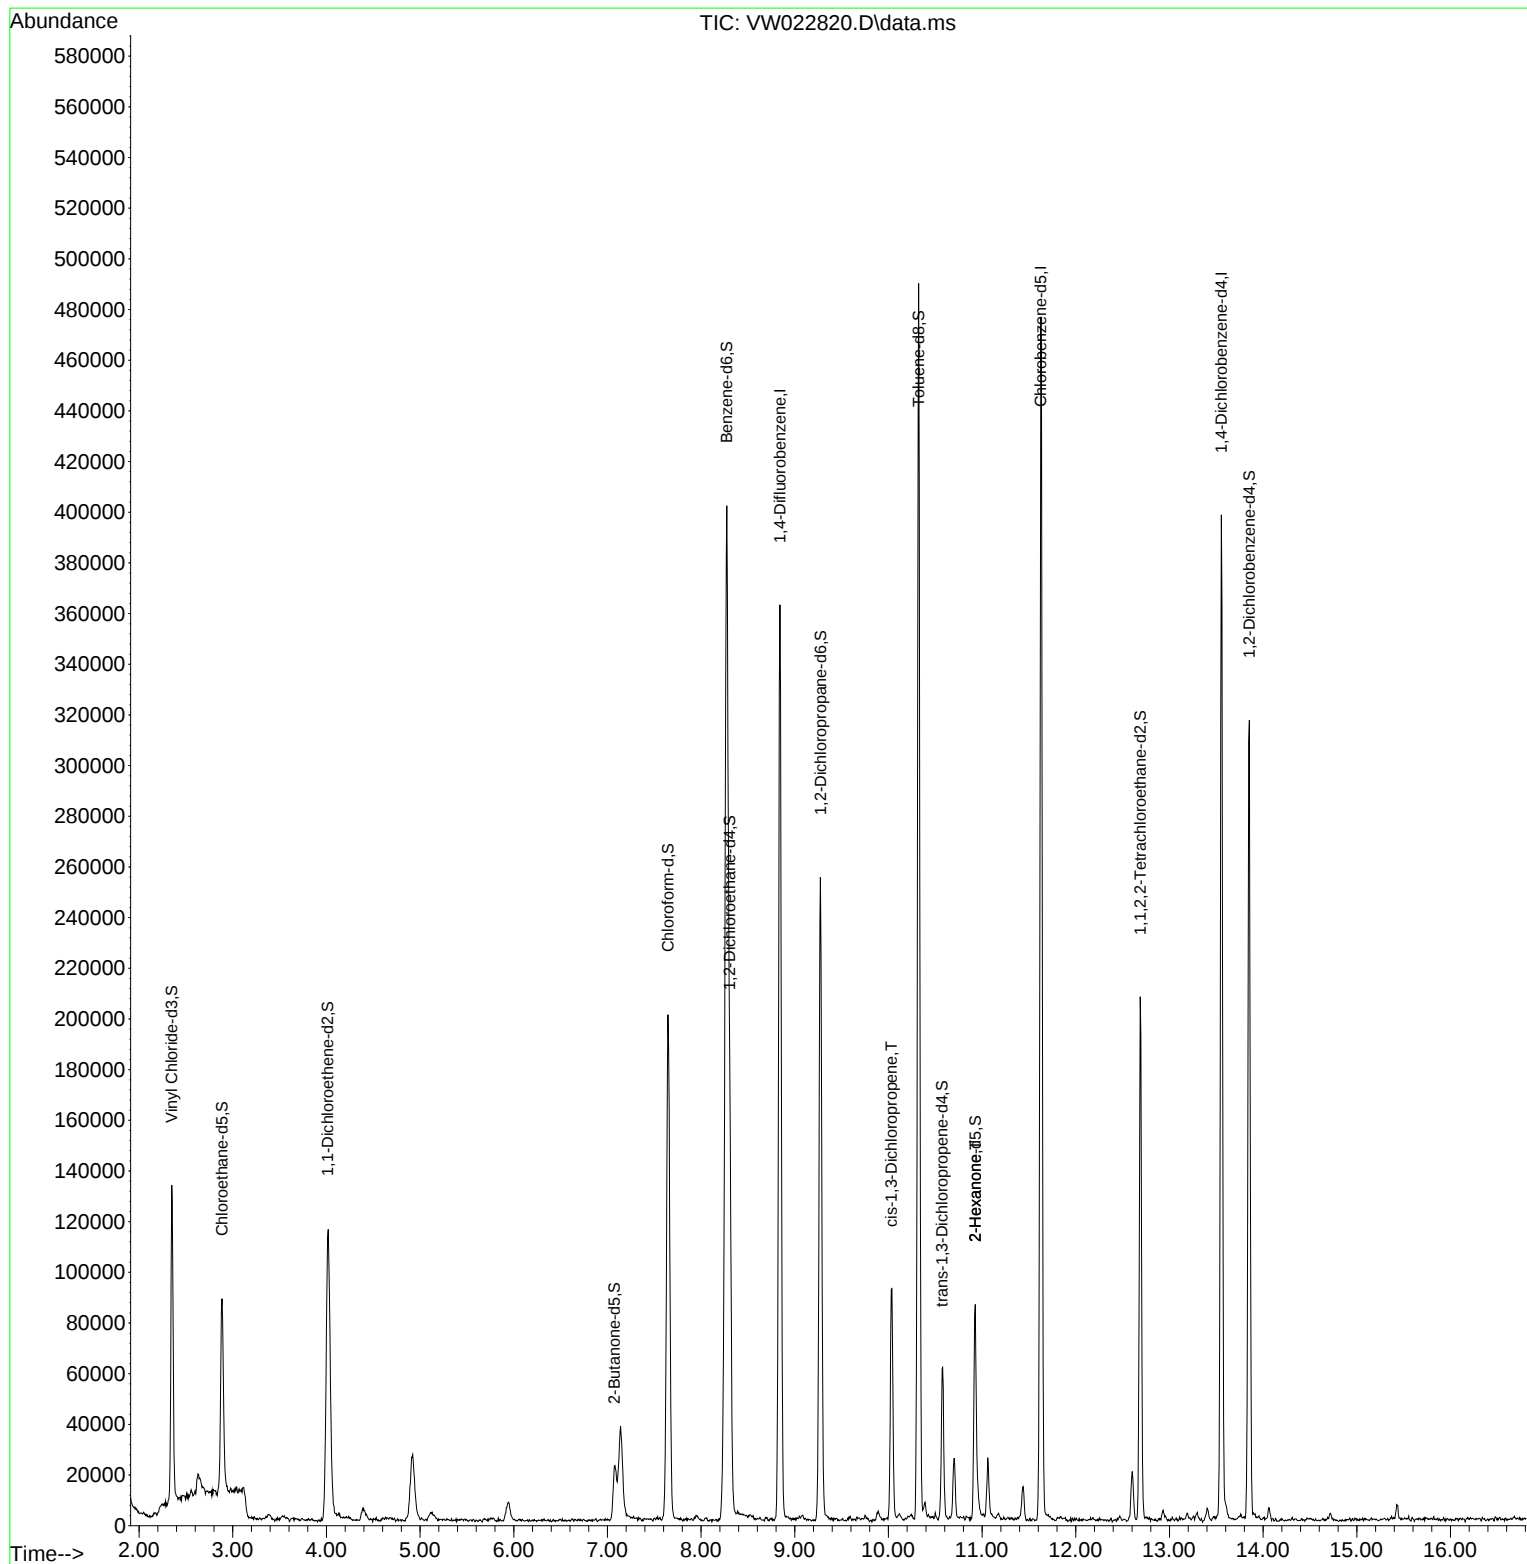

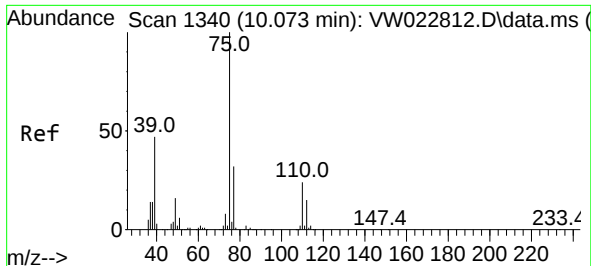

#39

cis-1,3-Dichloropropene

Concen: 0.627 ug/L

RT: 10.030 min Scan# 11

Delta R.T. -0.043 min

Lab File: VW022820.D

Acq: 04 May 2022 23:26

Instrument :

MSVOA_W

ClientSampleId :





BGBQ9

Tgt Ion: 75 Resp: 3521

Ion Ratio Lower Upper

75 100

77 33.9 22.1 41.1

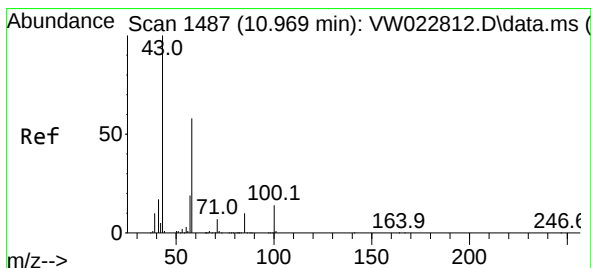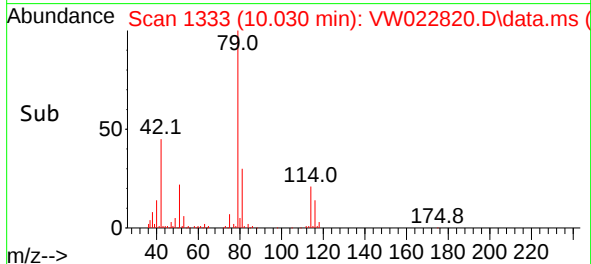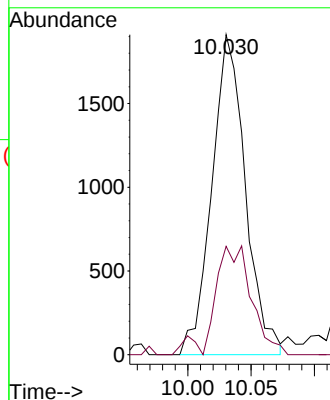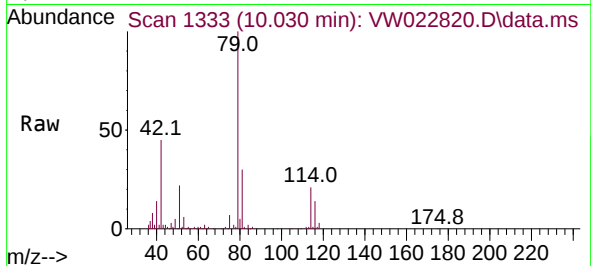

#48

2-Hexanone

Concen: 2.278 ug/L

RT: 10.926 min Scan# 1480

Delta R.T. -0.043 min

Lab File: VW022820.D

Acq: 04 May 2022 23:26

Tgt Ion: 43 Resp: 3473

Ion Ratio Lower Upper

43 100

58 33.5 45.9 68.9#

57 35.2 16.2 24.2#

100 4.5 10.7 16.1#

