




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022792.D
 Acq On : 04 May 2022 11:16
 Operator : SY/VA
 Sample : N2632-04RE
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A5RE

Manual IntegrationsAPPROVED

Quant Time: May 04 23:35:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

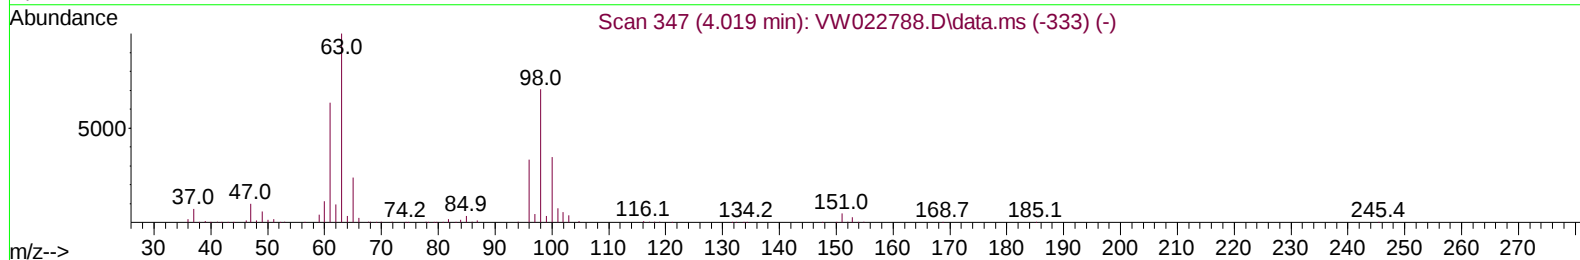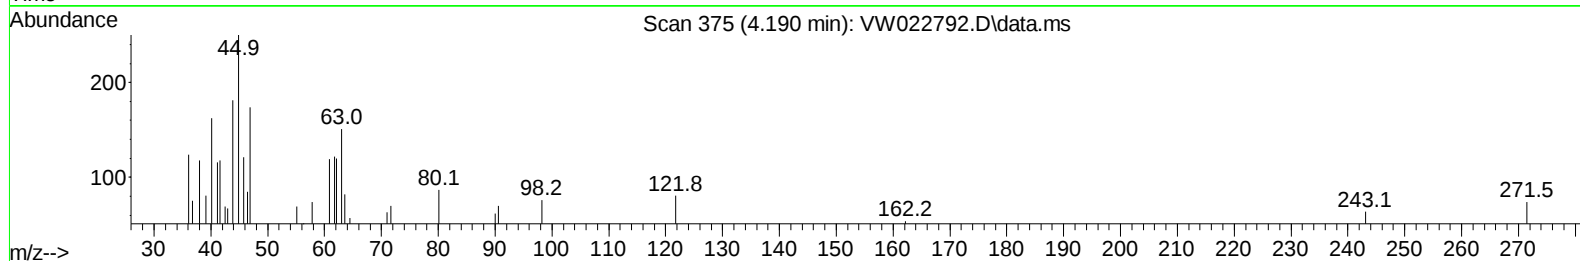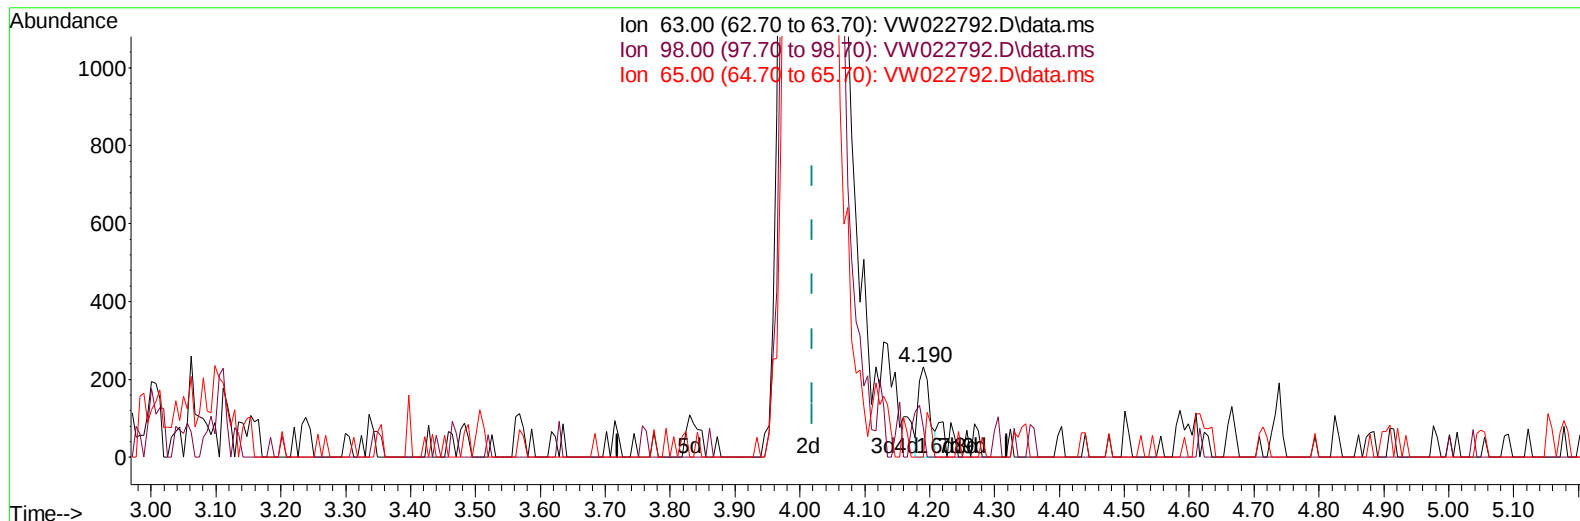

TIC: VW022792.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.190min (+ 0.171) 0.04 ug/L

response 284

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	51.41
65.00	23.30	25.70
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022792.D
 Acq On : 04 May 2022 11:16
 Operator : SY/VA
 Sample : N2632-04RE
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A5RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:35:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

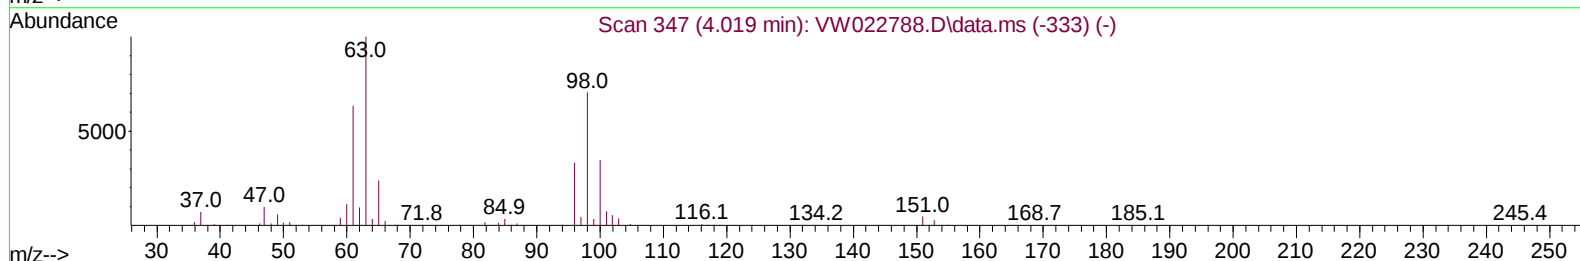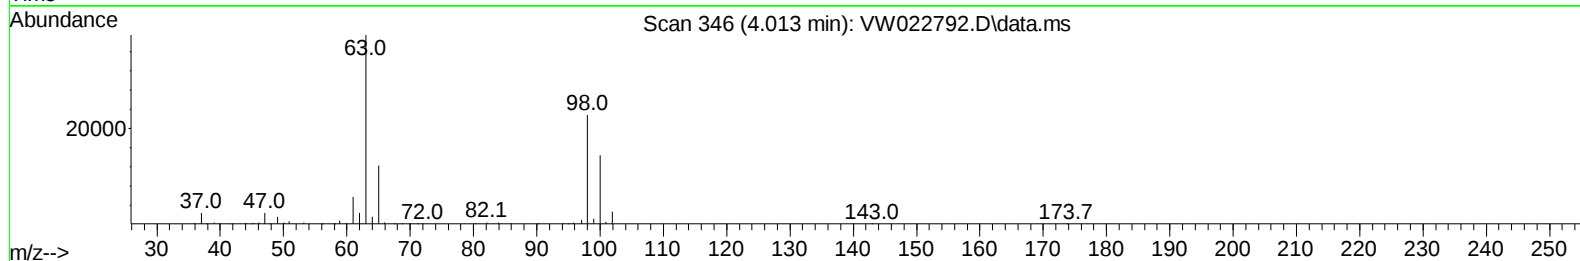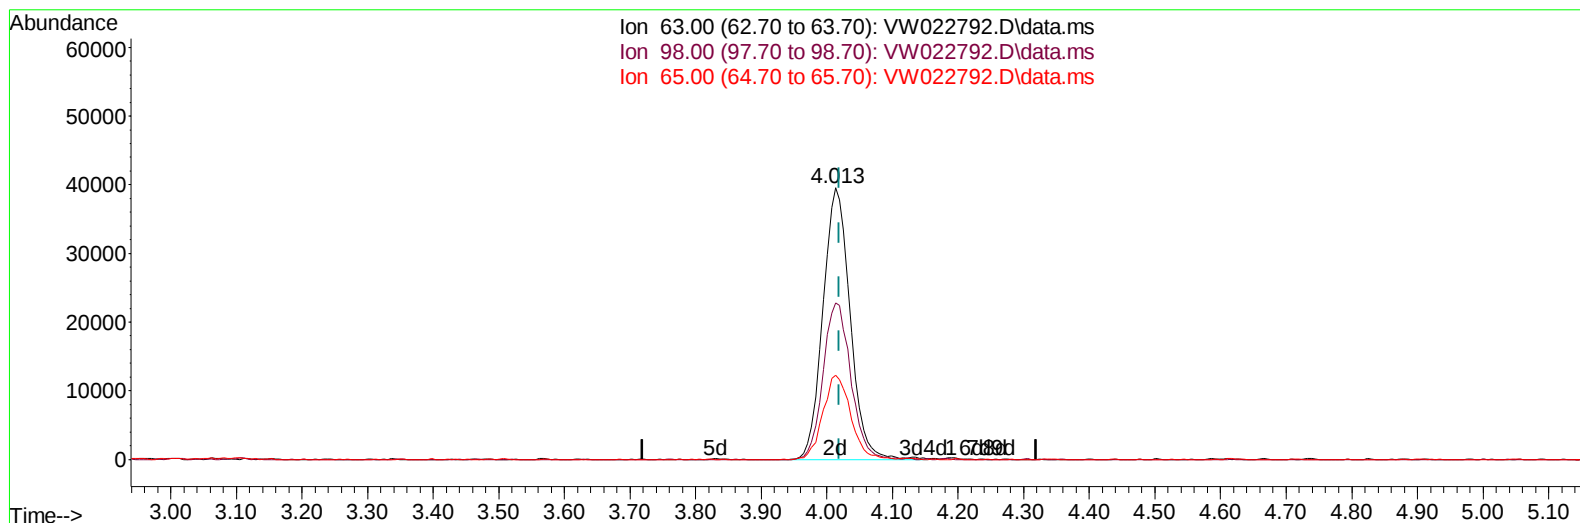

TIC: VW022792.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 16.66 ug/L m

response 113845

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.13#
65.00	23.30	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022792.D
 Acq On : 04 May 2022 11:16
 Operator : SY/VA
 Sample : N2632-04RE
 Misc : 6.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A5RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:35:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	257745	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	211176	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	69468	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	121773	23.028	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.120%	
7) Chloroethane-d5	2.879	69	83157	24.172	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.680%	
11) 1,1-Dichloroethene-d2	4.013	63	113845m	16.662	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.640%	
21) 2-Butanone-d5	7.074	46	62225	61.890	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	123.780%	
24) Chloroform-d	7.647	84	181065	23.978	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.920%	
26) 1,2-Dichloroethane-d4	8.305	65	111808	26.996	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	108.000%	
32) Benzene-d6	8.275	84	346866	28.497	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	114.000%	
36) 1,2-Dichloropropane-d6	9.274	67	102851	30.081	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	120.320%#	
41) Toluene-d8	10.323	98	295203	25.106	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	100.440%	
43) trans-1,3-Dichloroprop...	10.579	79	40777	25.901	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	103.600%	
47) 2-Hexanone-d5	10.920	63	51654	79.137	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	158.280%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103222	32.390	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	129.560%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	61048	25.140	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.560%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022792.D
Acq On : 04 May 2022 11:16
Operator : SY/VA
Sample : N2632-04RE
Misc : 6.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4A5RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:35:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

