




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022794.D
 Acq On : 04 May 2022 12:04
 Operator : SY/VA
 Sample : N2632-06RE
 Misc : 6.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A7RE

Manual IntegrationsAPPROVED

Quant Time: May 04 23:35:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

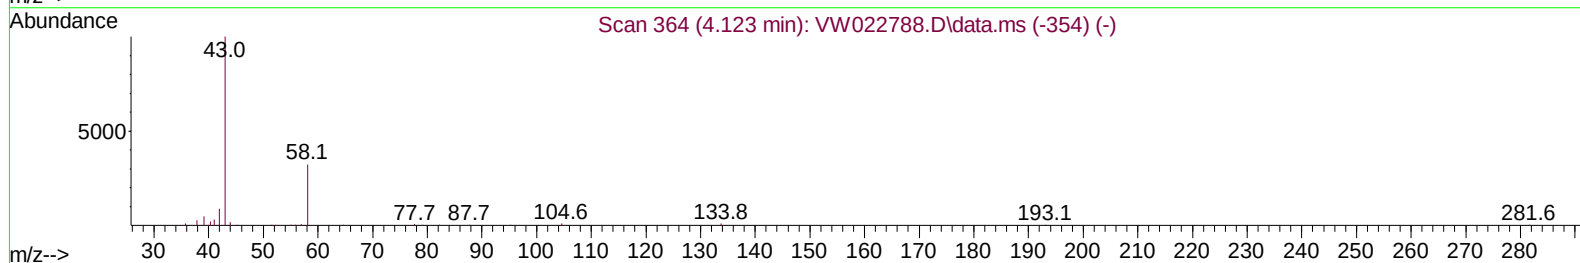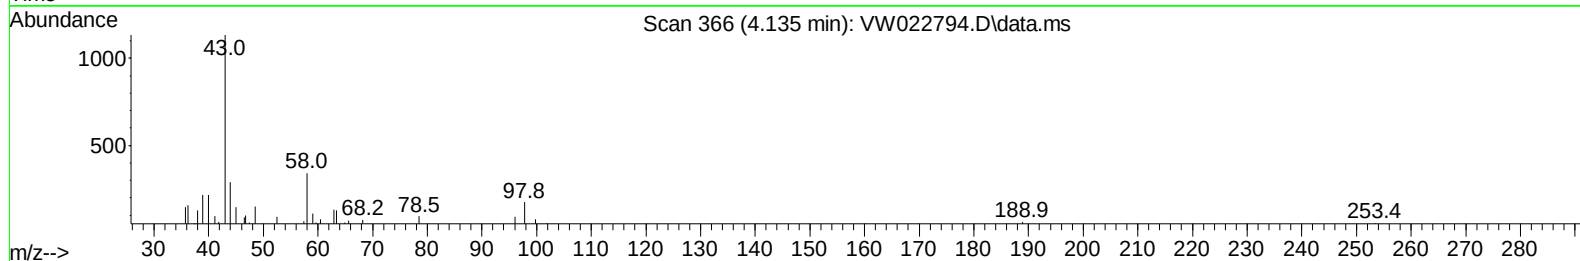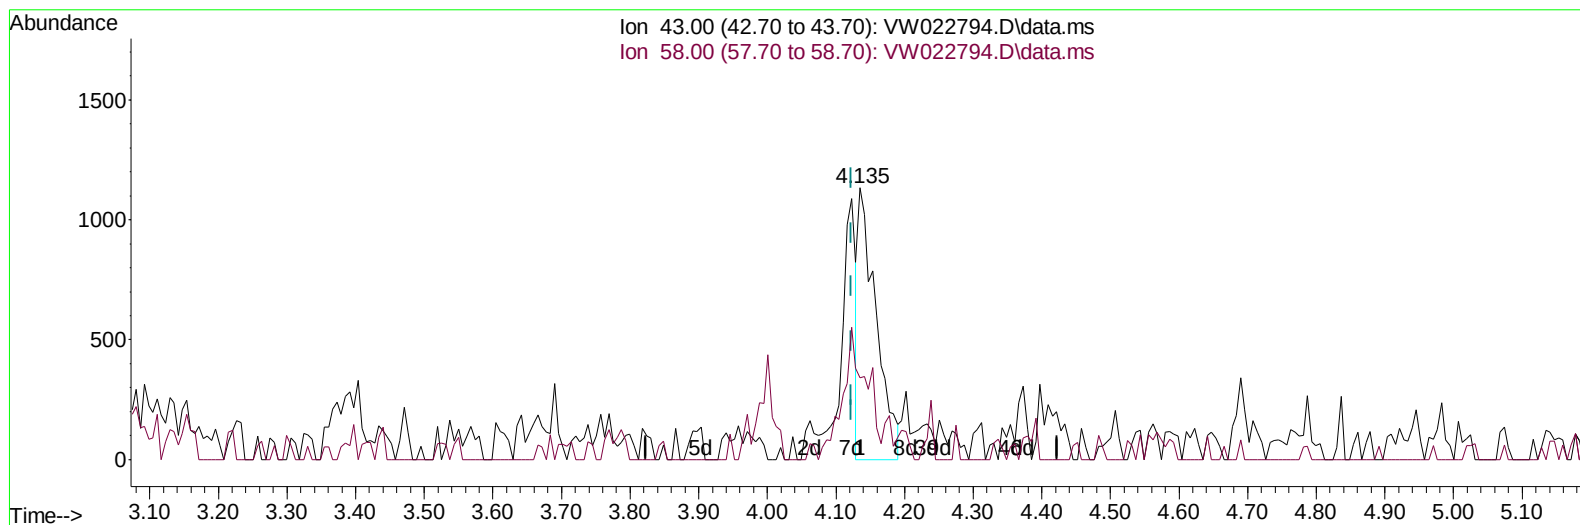

TIC: VW022794.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 2.56 ug/L

response 2031

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	10.44
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022794.D
 Acq On : 04 May 2022 12:04
 Operator : SY/VA
 Sample : N2632-06RE
 Misc : 6.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A7RE

Manual IntegrationsAPPROVED

Quant Time: May 04 23:35:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

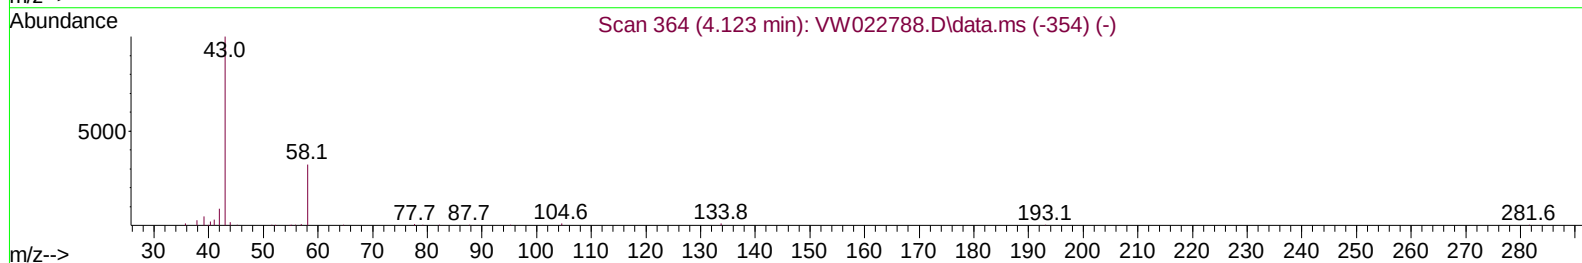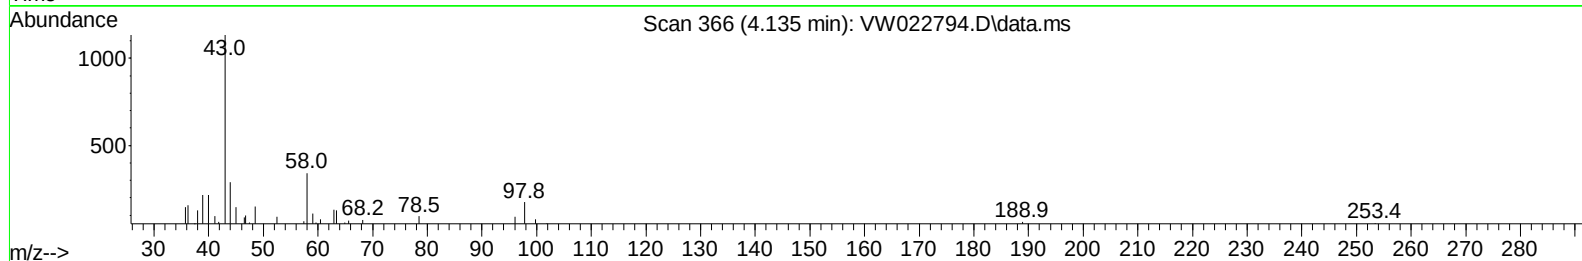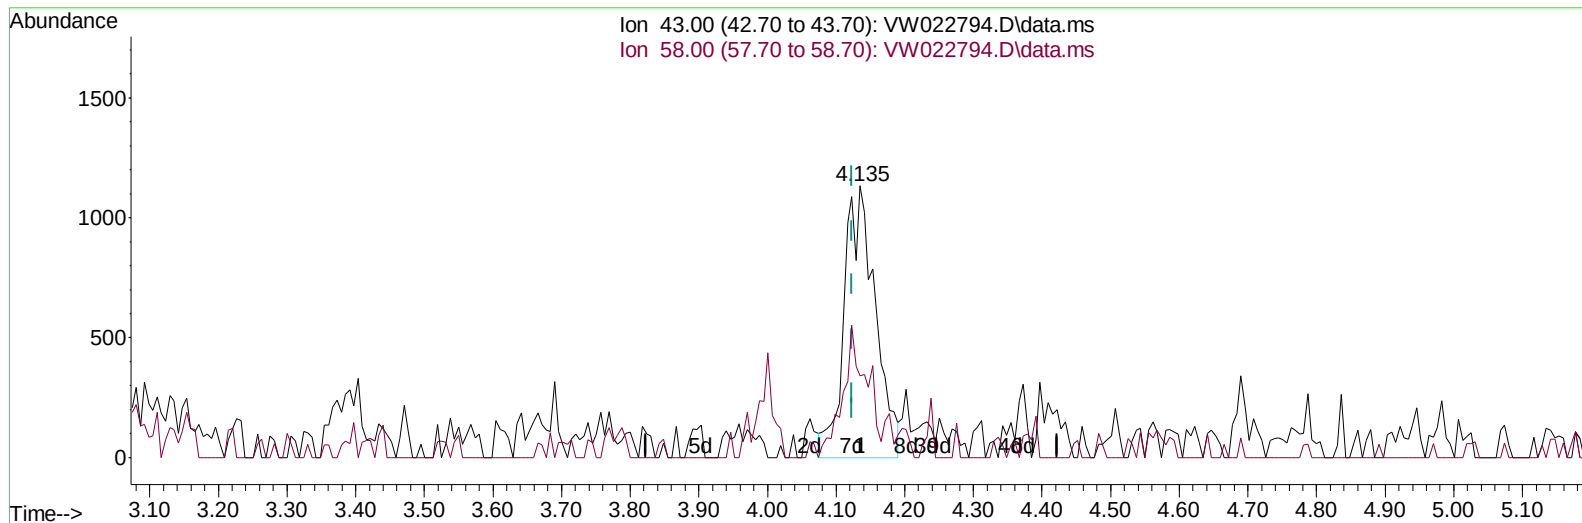

TIC: VW022794.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 4.51 ug/L m

response 3575

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	5.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022794.D
 Acq On : 04 May 2022 12:04
 Operator : SY/VA
 Sample : N2632-06RE
 Misc : 6.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4A7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:35:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	271544	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	203365	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	58443	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	136387	24.481	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	97.920%	
7) Chloroethane-d5	2.885	69	95872	26.451	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.800%	
11) 1,1-Dichloroethene-d2	4.019	63	115719	16.075	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	64.320%	
21) 2-Butanone-d5	7.080	46	52919	49.959	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	99.920%	
24) Chloroform-d	7.647	84	194515	24.450	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	8.305	65	107412	24.617	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	98.480%	
32) Benzene-d6	8.274	84	364433	31.090	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	124.360%	
36) 1,2-Dichloropropane-d6	9.274	67	108271	32.882	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	131.520%#	
41) Toluene-d8	10.323	98	292091	25.795	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	103.200%	
43) trans-1,3-Dichloroprop...	10.579	79	33353	21.999	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	88.000%	
47) 2-Hexanone-d5	10.920	63	37813	60.157	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.320%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	90640	29.534	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	118.120%	
66) 1,2-Dichlorobenzene-d4	13.853	152	63924	31.290	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	125.160%#	
Target Compounds						Qvalue
13) Acetone	4.135	43	3575m	4.508	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022794.D
Acq On : 04 May 2022 12:04
Operator : SY/VA
Sample : N2632-06RE
Misc : 6.80g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4A7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:35:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

