

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022797.D
 Acq On : 04 May 2022 13:17
 Operator : SY/VA
 Sample : N2632-11RE
 Misc : 6.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Dadoda 05/09/2022

Quant Time: May 04 23:36:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

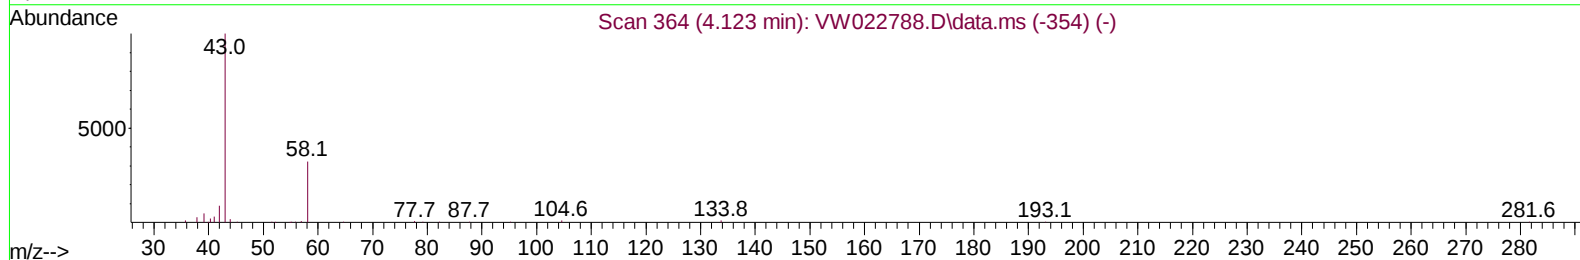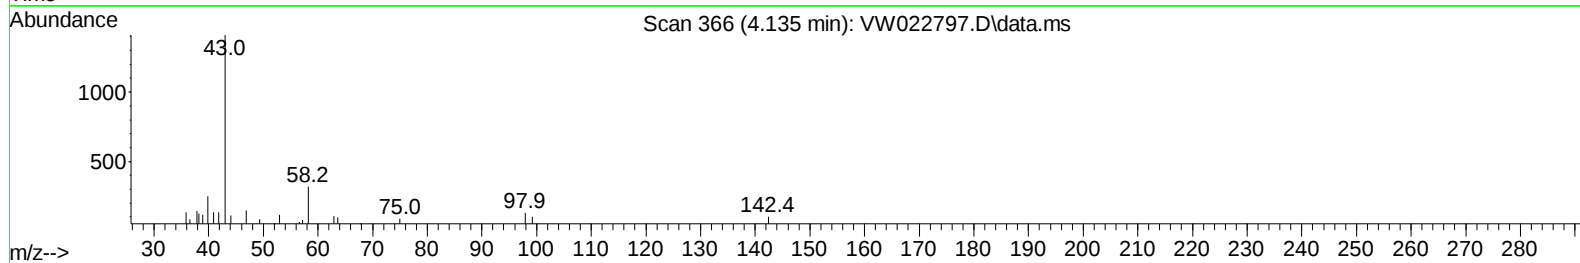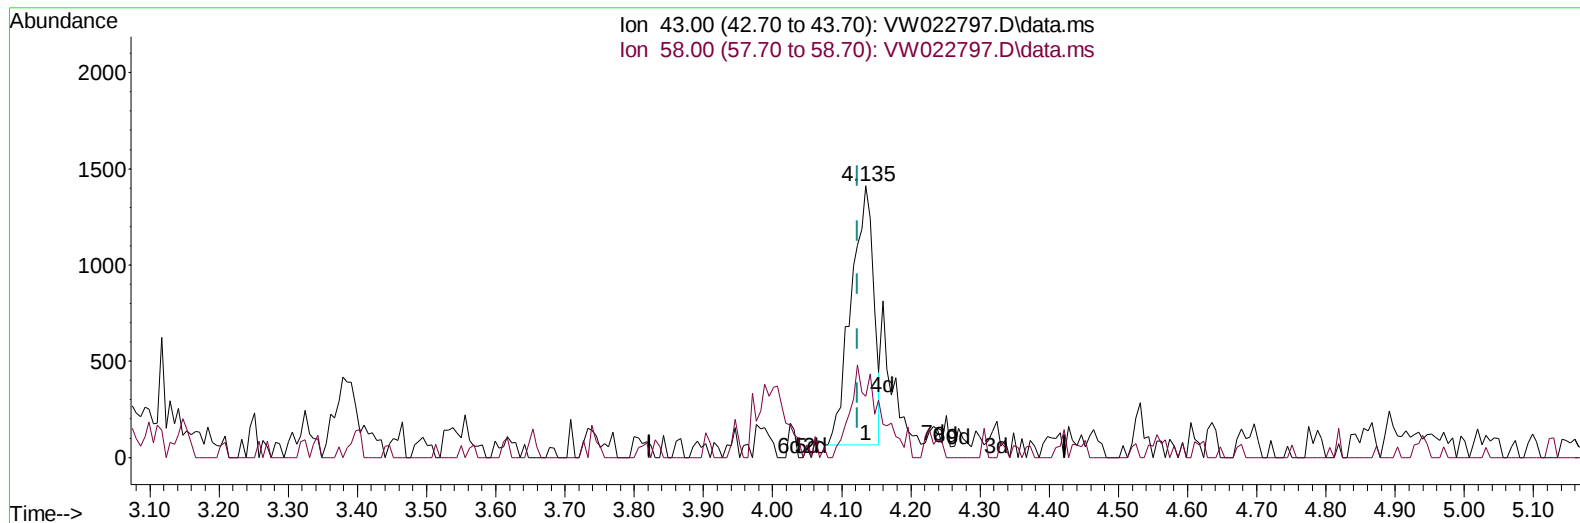

TIC: VW022797.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 5.27 ug/L

response 3054

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	15.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022797.D
 Acq On : 04 May 2022 13:17
 Operator : SY/VA
 Sample : N2632-11RE
 Misc : 6.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Dadoda 05/09/2022

Quant Time: May 04 23:36:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

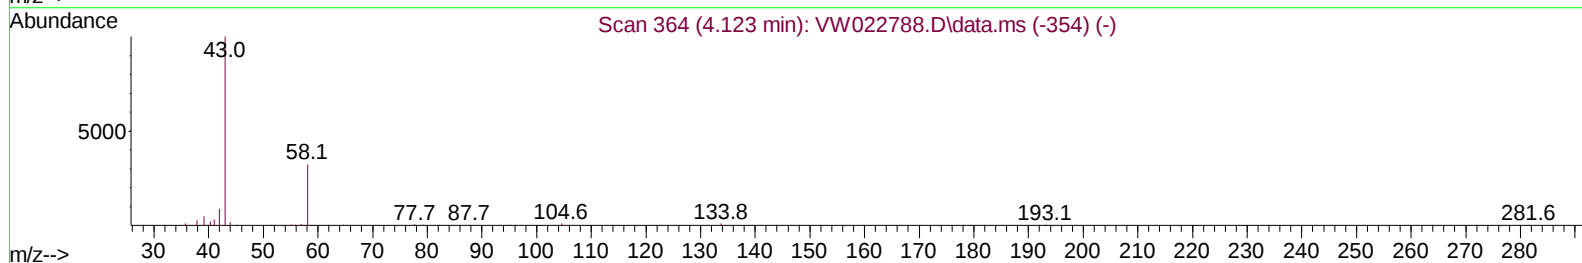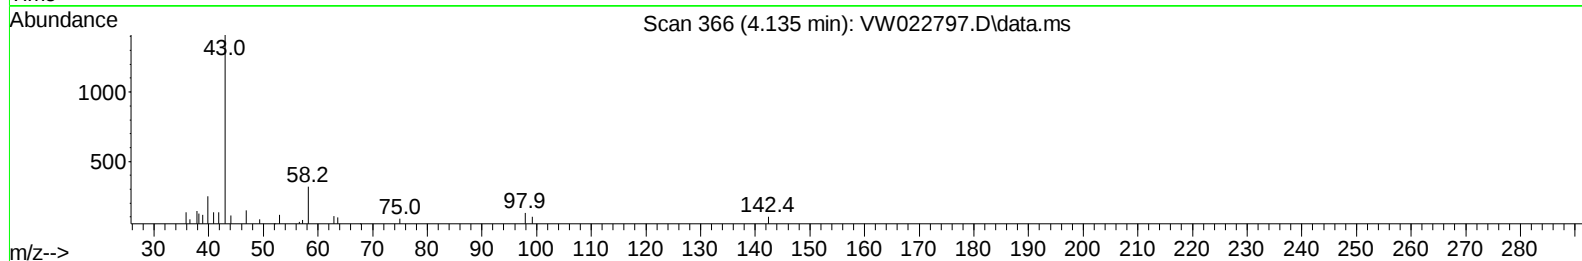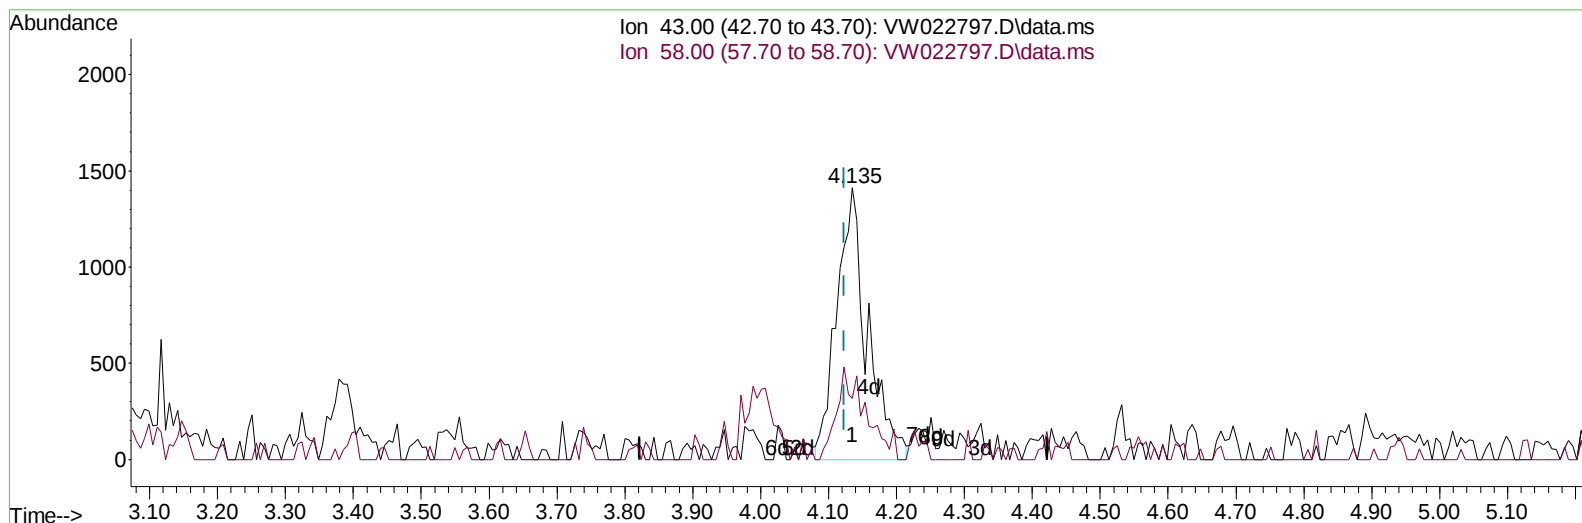

TIC: VW022797.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 7.57 ug/L m

response 4383

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	10.81
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022797.D
 Acq On : 04 May 2022 13:17
 Operator : SY/VA
 Sample : N2632-11RE
 Misc : 6.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Dadoda 05/09/2022

Quant Time: May 04 23:36:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		198307	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		108183	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		17854	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		110571	27.177	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	108.720%	
7) Chloroethane-d5	2.885	69		72086	27.234	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	108.920%	
11) 1,1-Dichloroethene-d2	4.019	63		87131	16.574	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	66.280%	
21) 2-Butanone-d5	7.080	46		52905	68.391	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	136.780%#	
24) Chloroform-d	7.653	84		155494	26.763	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	107.040%	
26) 1,2-Dichloroethane-d4	8.305	65		89918	28.218	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	112.880%	
32) Benzene-d6	8.275	84		276552	44.351	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	177.400%#	
36) 1,2-Dichloropropane-d6	9.274	67		89735	51.230	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	204.920%#	
41) Toluene-d8	10.323	98		186834	31.017	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	124.080%	
43) trans-1,3-Dichloroprop...	10.579	79		21985	27.260	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	109.040%	
47) 2-Hexanone-d5	10.920	63		36800	110.055	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	220.120%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		79764	48.857	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	195.440%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		23209	37.187	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	148.760%#	
Target Compounds							
13) Acetone	4.135	43		4383m	7.568	ug/L	
42) Toluene	10.384	91		9238	1.293	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022797.D
Acq On : 04 May 2022 13:17
Operator : SY/VA
Sample : N2632-11RE
Misc : 6.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4B3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Dadoda 05/09/2022

Quant Time: May 04 23:36:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

