




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022800.D
Acq On : 04 May 2022 14:29
Operator : SY/VA
Sample : N2632-15RE
Misc : 7.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4B7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:36:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

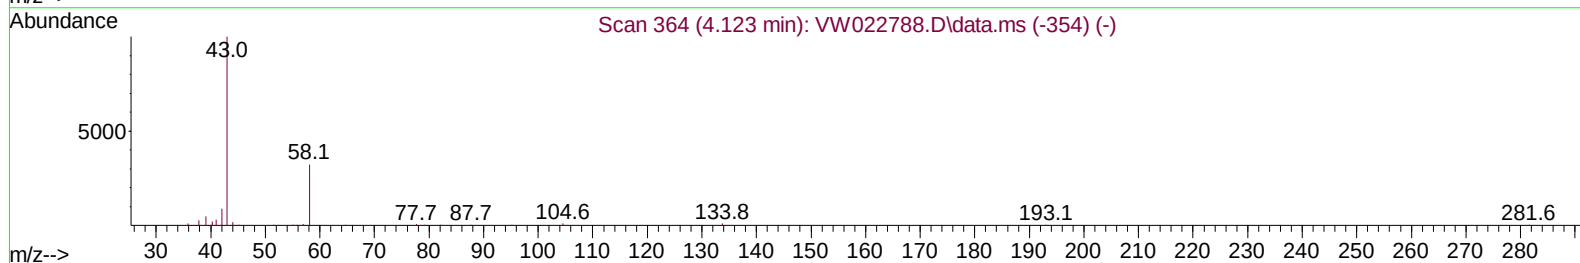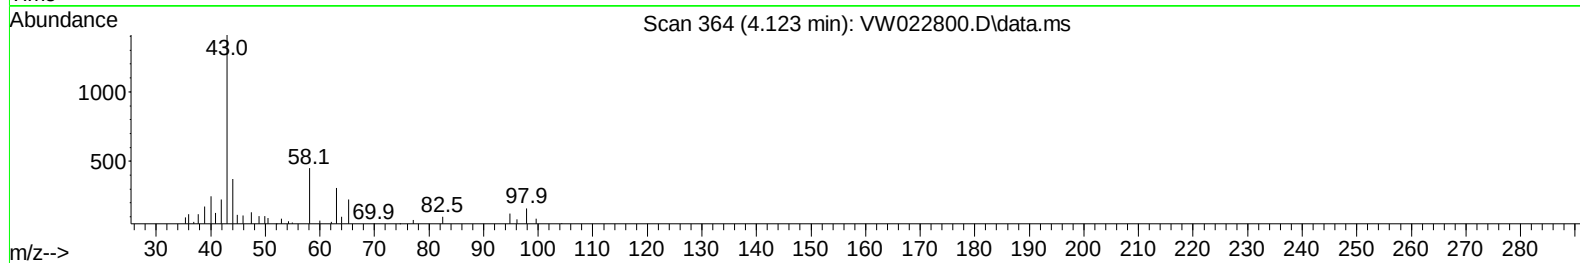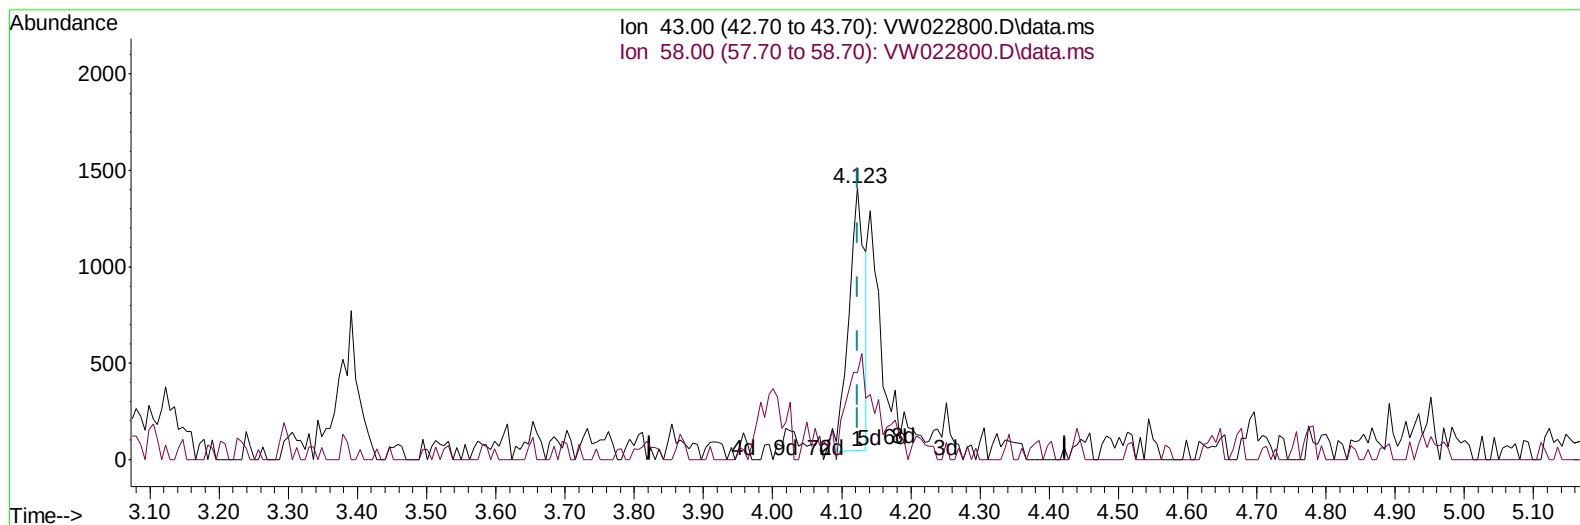

TIC: VW022800.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 2.65 ug/L

response 2171

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	61.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022800.D
 Acq On : 04 May 2022 14:29
 Operator : SY/VA
 Sample : N2632-15RE
 Misc : 7.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B7RE

Manual IntegrationsAPPROVED

Quant Time: May 04 23:36:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

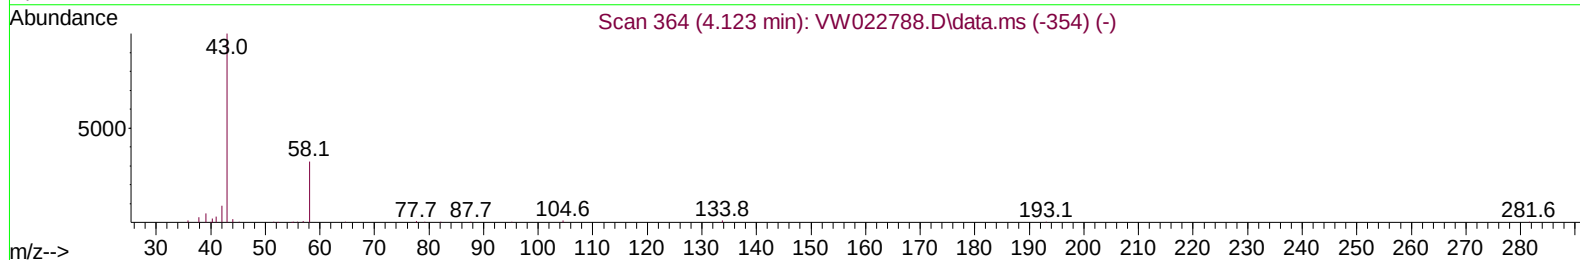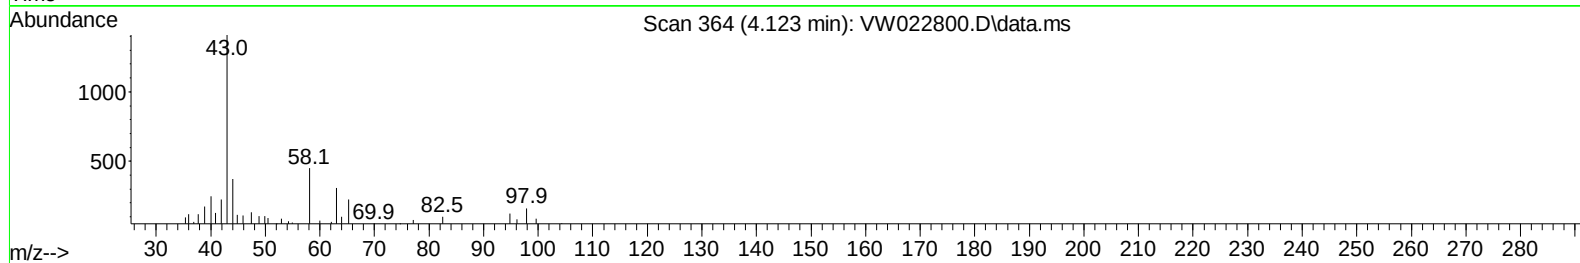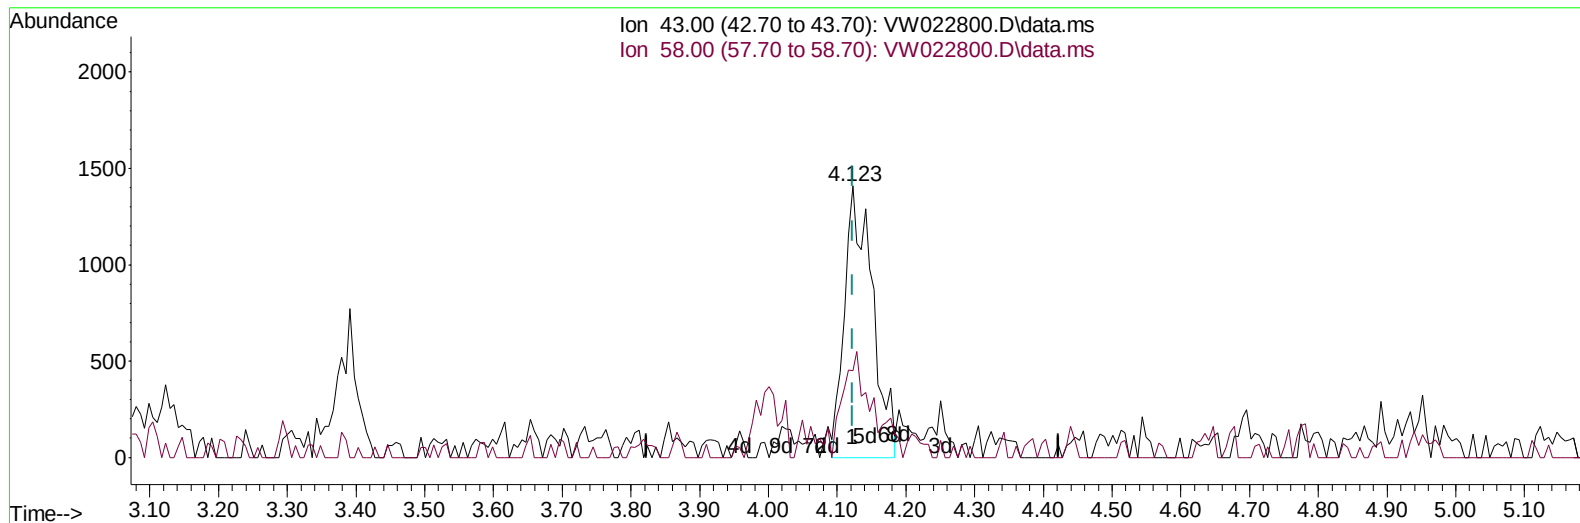

TIC: VW022800.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 4.81 ug/L m

response 3952

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	33.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022800.D
 Acq On : 04 May 2022 14:29
 Operator : SY/VA
 Sample : N2632-15RE
 Misc : 7.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4B7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:36:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		281042	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		182182	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		36450	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		149925	26.002	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	104.000%	
7) Chloroethane-d5	2.885	69		108122	28.823	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	115.280%	
11) 1,1-Dichloroethene-d2	4.013	63		129438	17.374	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	69.480%	
21) 2-Butanone-d5	7.074	46		60848	55.503	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	111.000%	
24) Chloroform-d	7.647	84		212158	25.766	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	103.080%	
26) 1,2-Dichloroethane-d4	8.305	65		113590	25.153	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	100.600%	
32) Benzene-d6	8.275	84		387217	36.875	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	147.480%#	
36) 1,2-Dichloropropane-d6	9.274	67		114826	38.928	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	155.720%#	
41) Toluene-d8	10.323	98		295256	29.107	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	116.440%	
43) trans-1,3-Dichloroprop...	10.579	79		33383	24.579	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	98.320%	
47) 2-Hexanone-d5	10.920	63		40214	71.416	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	142.840%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		86465	31.449	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	125.800%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		38483	30.202	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	120.800%#	
Target Compounds							
13) Acetone	4.123	43		3952m	4.815	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022800.D
Acq On : 04 May 2022 14:29
Operator : SY/VA
Sample : N2632-15RE
Misc : 7.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4B7RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:36:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

