




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022810.D
Acq On : 04 May 2022 18:30
Operator : SY/VA
Sample : VIBLK445
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK445

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:38:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

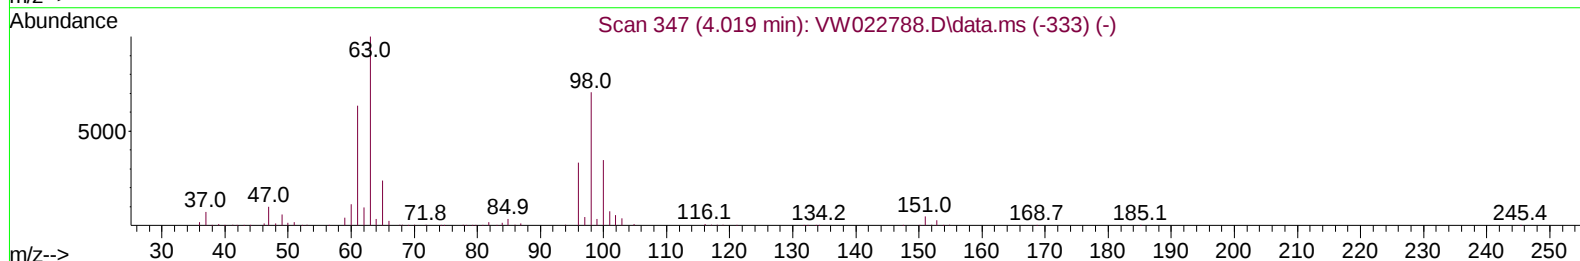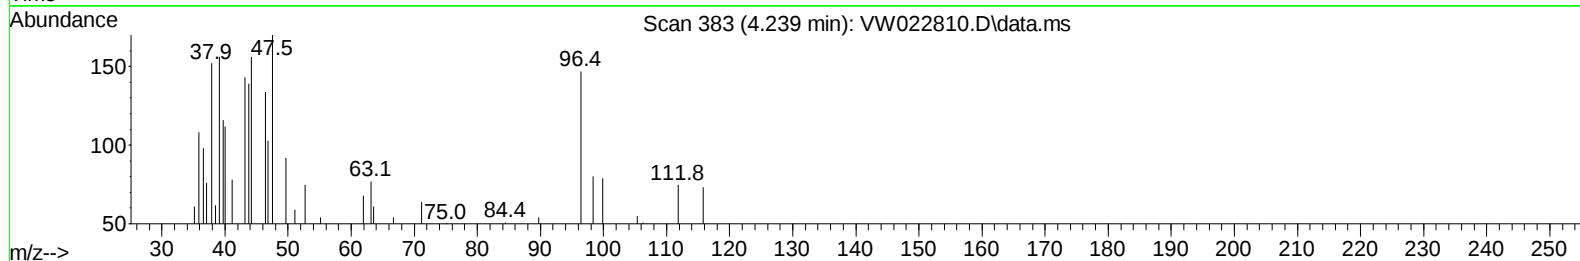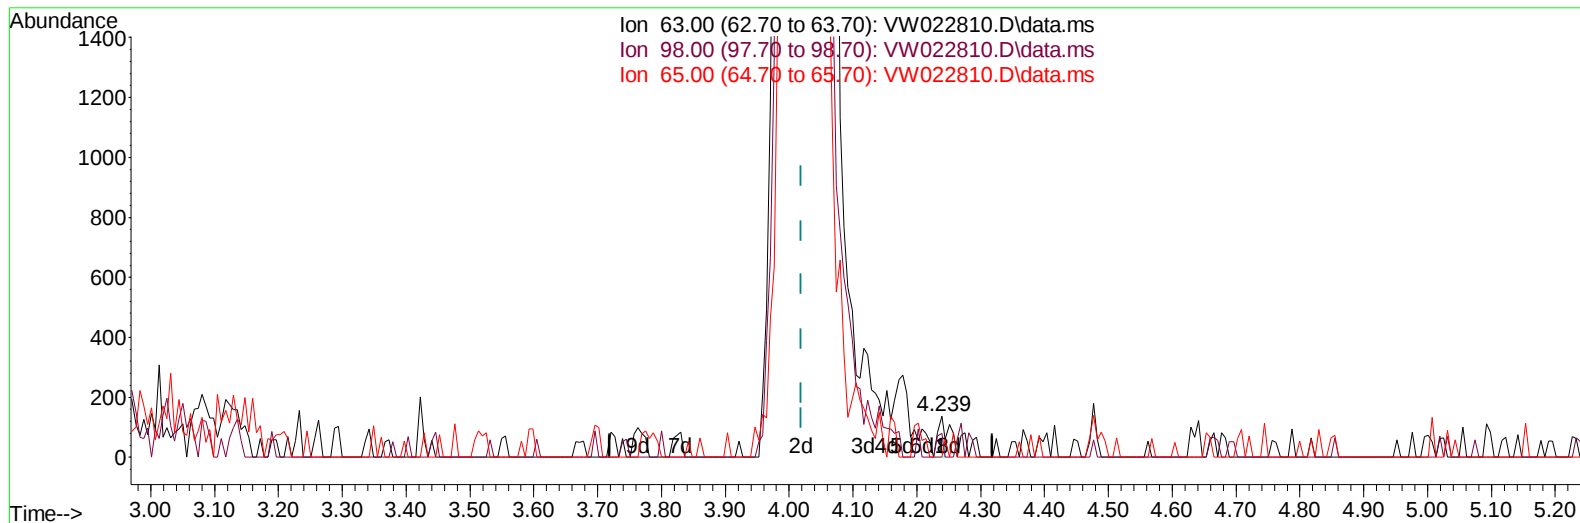

TIC: VW022810.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.239min (+ 0.220) 0.01 ug/L

response 103

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	53.40
65.00	23.30	21.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022810.D
Acq On : 04 May 2022 18:30
Operator : SY/VA
Sample : VIBLK445
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK445

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:38:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

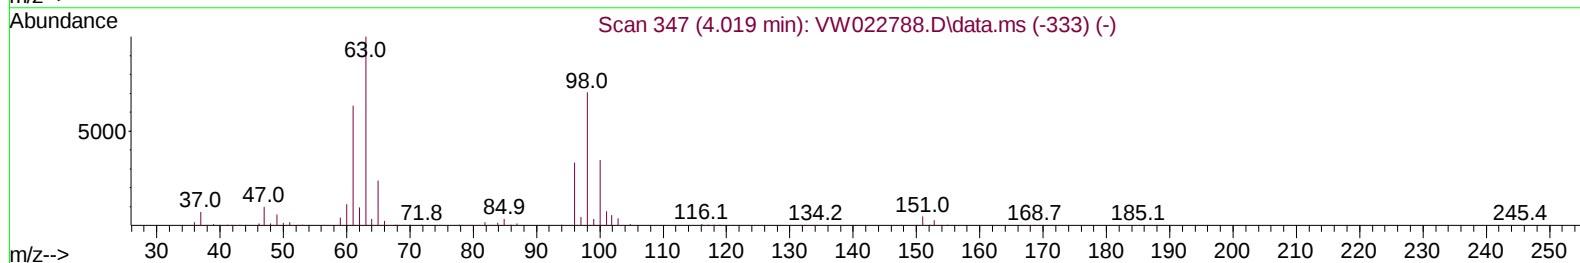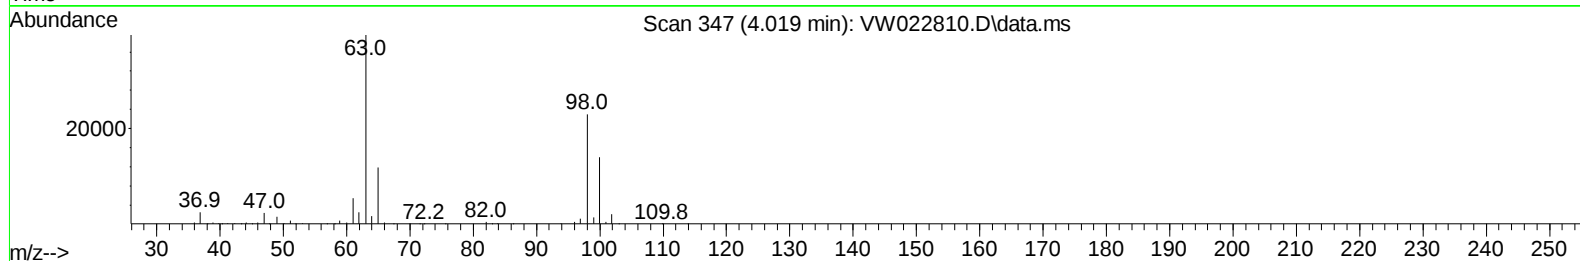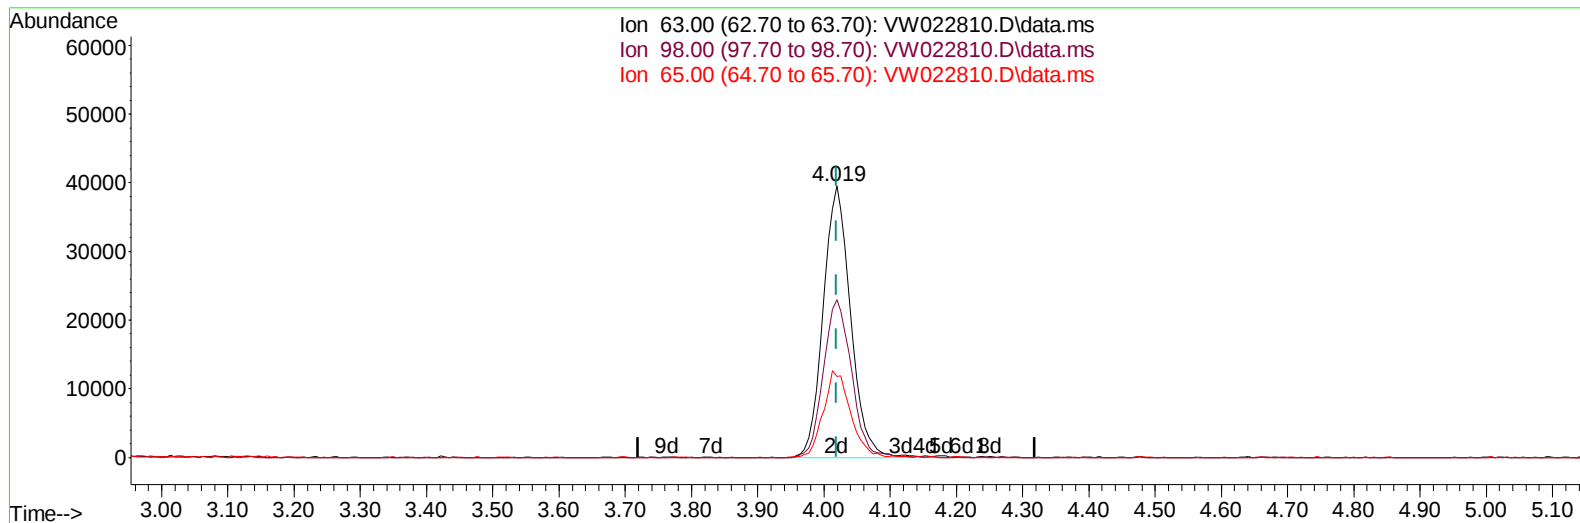

TIC: VW022810.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (+ 0.000) 14.49 ug/L m

response 113331

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.05#
65.00	23.30	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022810.D
 Acq On : 04 May 2022 18:30
 Operator : SY/VA
 Sample : VIBLK445
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK445

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:38:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		295066	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		294834	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		151668	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		119907	19.807	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.240%		
7) Chloroethane-d5	2.885	69		89135	22.632	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	90.520%		
11) 1,1-Dichloroethene-d2	4.019	63		113331m	14.489	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.960%		
21) 2-Butanone-d5	7.074	46		50655	44.009	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	88.020%		
24) Chloroform-d	7.653	84		185251	21.429	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	85.720%		
26) 1,2-Dichloroethane-d4	8.305	65		105850	22.325	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	89.320%		
32) Benzene-d6	8.274	84		363320	21.379	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	85.520%		
36) 1,2-Dichloropropane-d6	9.274	67		106935	22.401	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	89.600%		
41) Toluene-d8	10.323	98		338984	20.649	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.600%		
43) trans-1,3-Dichloroprop...	10.573	79		40756	18.542	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	74.160%		
47) 2-Hexanone-d5	10.920	63		39603	43.458	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	86.920%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		96067	21.591	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	86.360%		
66) 1,2-Dichlorobenzene-d4	13.853	152		113571	21.421	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	85.680%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022810.D
Acq On : 04 May 2022 18:30
Operator : SY/VA
Sample : VIBLK445
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK445

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:38:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

