




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022811.D
 Acq On : 04 May 2022 18:54
 Operator : SY/VA
 Sample : N2638-02
 Misc : 5.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXKZ3

Manual IntegrationsAPPROVED

Quant Time: May 04 23:38:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

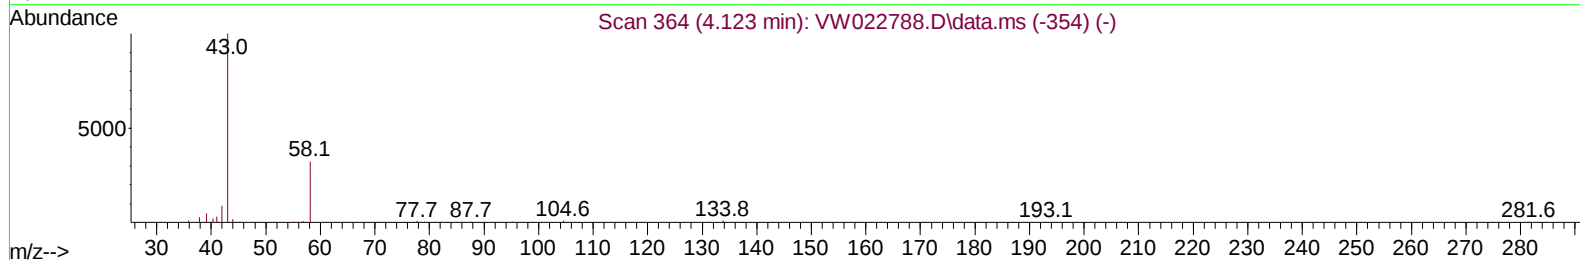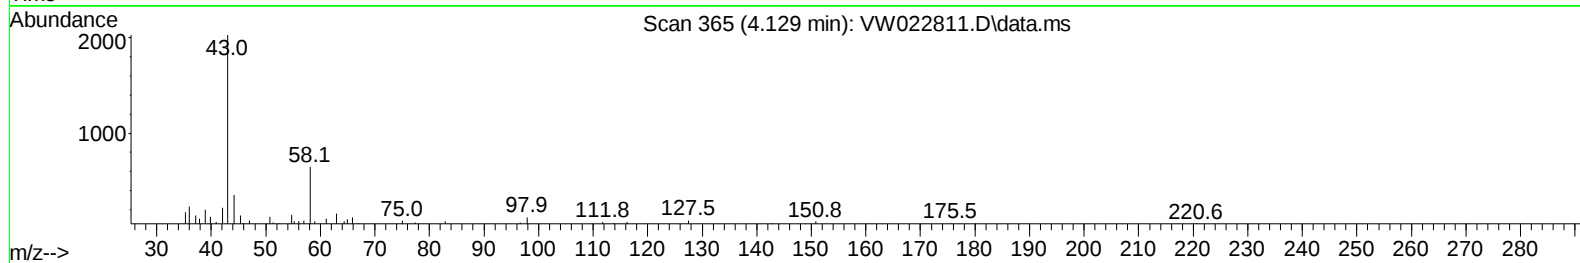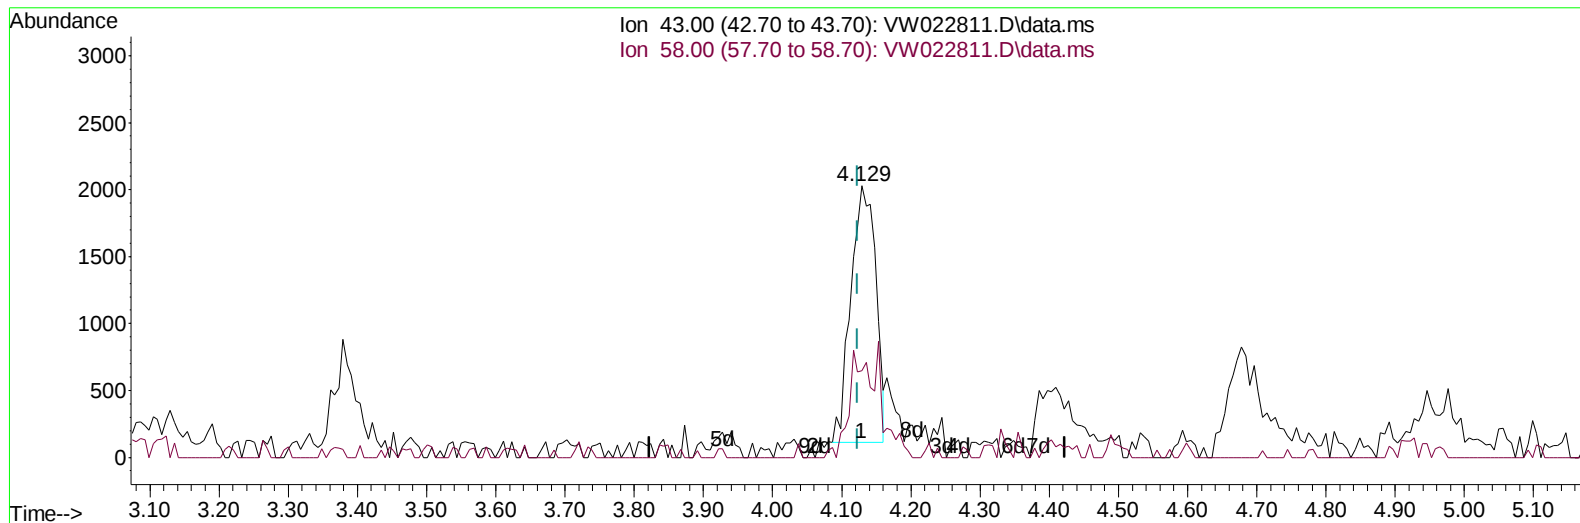

TIC: VW022811.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 4.84 ug/L

response 4811

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	18.02
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022811.D
 Acq On : 04 May 2022 18:54
 Operator : SY/VA
 Sample : N2638-02
 Misc : 5.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXKZ3

Manual IntegrationsAPPROVED

Quant Time: May 04 23:38:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

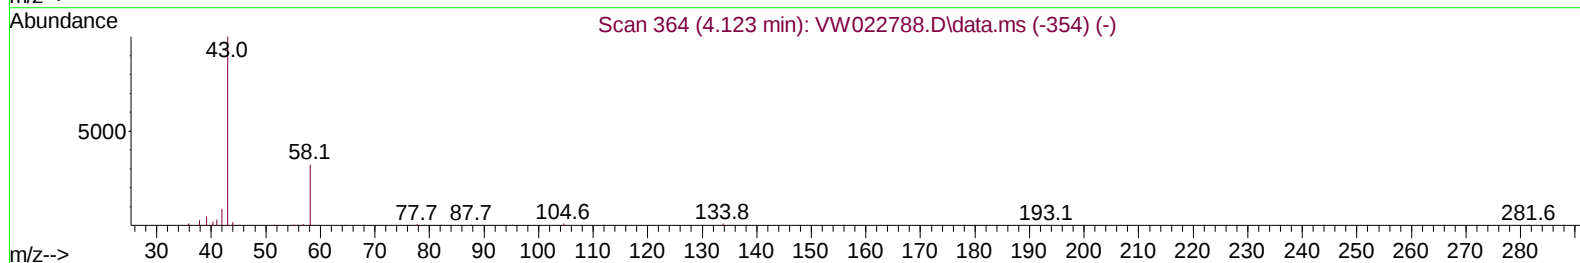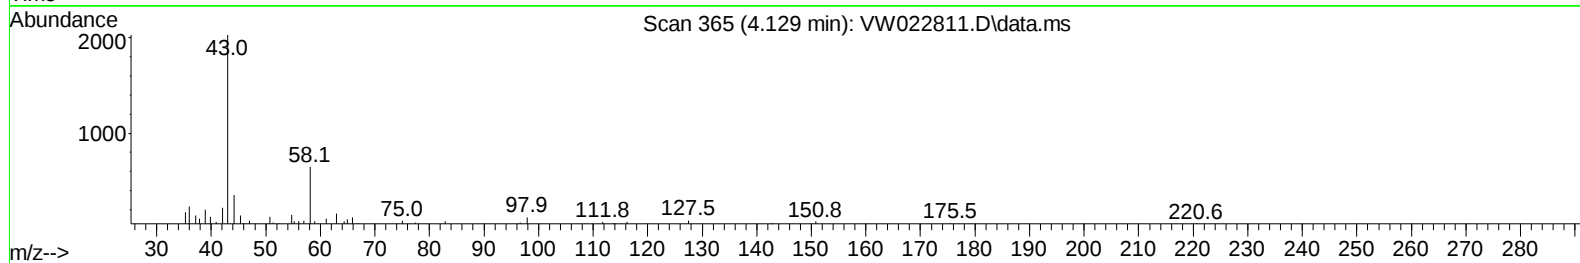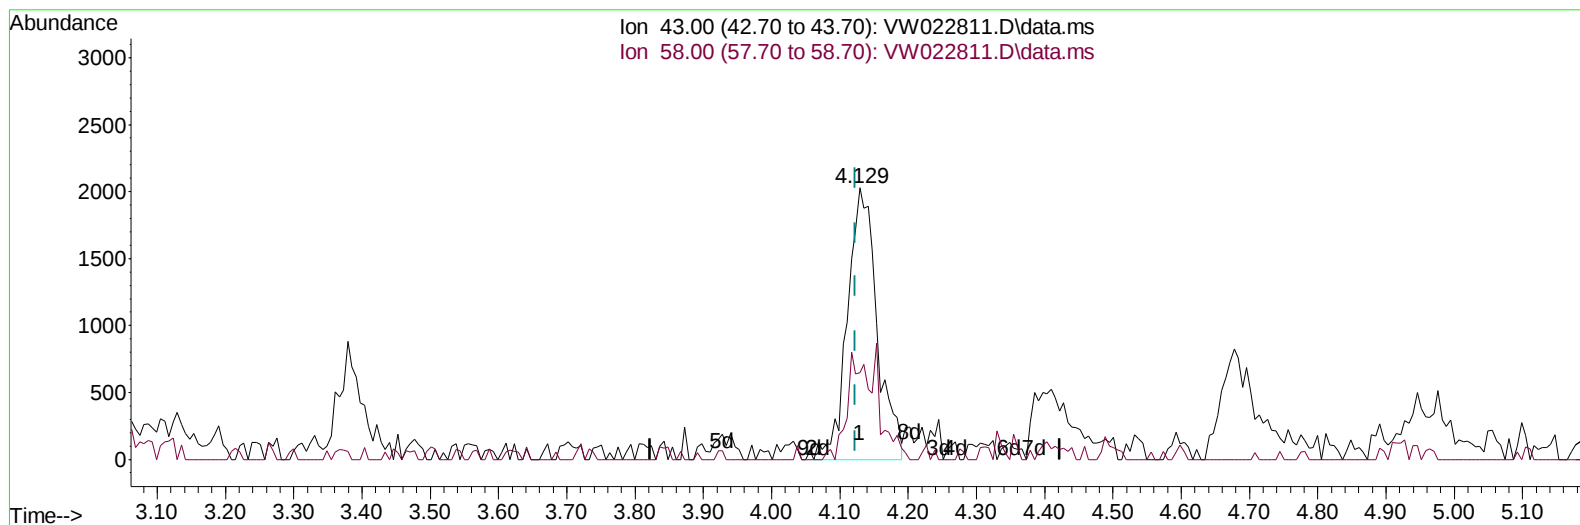

TIC: VW022811.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 6.16 ug/L m

response 6125

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	14.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
 Data File : VW022811.D
 Acq On : 04 May 2022 18:54
 Operator : SY/VA
 Sample : N2638-02
 Misc : 5.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EXKZ3

Manual IntegrationsAPPROVED

Quant Time: May 04 23:38:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 04 23:28:03 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/05/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	340343	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	322645	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	156269	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	137028	19.624	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	78.480%	
7) Chloroethane-d5	2.885	69	99303	21.860	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.440%	
11) 1,1-Dichloroethene-d2	4.013	63	124051	13.749	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.000%	
21) 2-Butanone-d5	7.080	46	54316	40.912	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	81.820%	
24) Chloroform-d	7.647	84	210058	21.066	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	84.280%	
26) 1,2-Dichloroethane-d4	8.305	65	120344	22.005	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	88.040%	
32) Benzene-d6	8.275	84	402457	21.641	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	86.560%	
36) 1,2-Dichloropropane-d6	9.274	67	121978	23.350	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	93.400%	
41) Toluene-d8	10.323	98	372595	20.740	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	82.960%	
43) trans-1,3-Dichloroprop...	10.579	79	46200	19.207	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	76.840%	
47) 2-Hexanone-d5	10.927	63	43310	43.430	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	86.860%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	101041	20.752	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	83.000%	
66) 1,2-Dichlorobenzene-d4	13.853	152	110230	20.179	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	80.720%	
Target Compounds						
13) Acetone	4.129	43	6125m	6.162	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW050422\
Data File : VW022811.D
Acq On : 04 May 2022 18:54
Operator : SY/VA
Sample : N2638-02
Misc : 5.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EXKZ3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/05/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 04 23:38:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 04 23:28:03 2022
Response via : Initial Calibration

